

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/20/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 00:28 |
| INTERNAL STANDARD | VERIFIED | 00:28 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 00:28 |
| BLANK TEST | 0.00 | 00:29 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 00:29 |
| BLANK TEST | 0.00 | 00:30 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 00:31 |
| BLANK TEST | 0.00 | 00:32 |

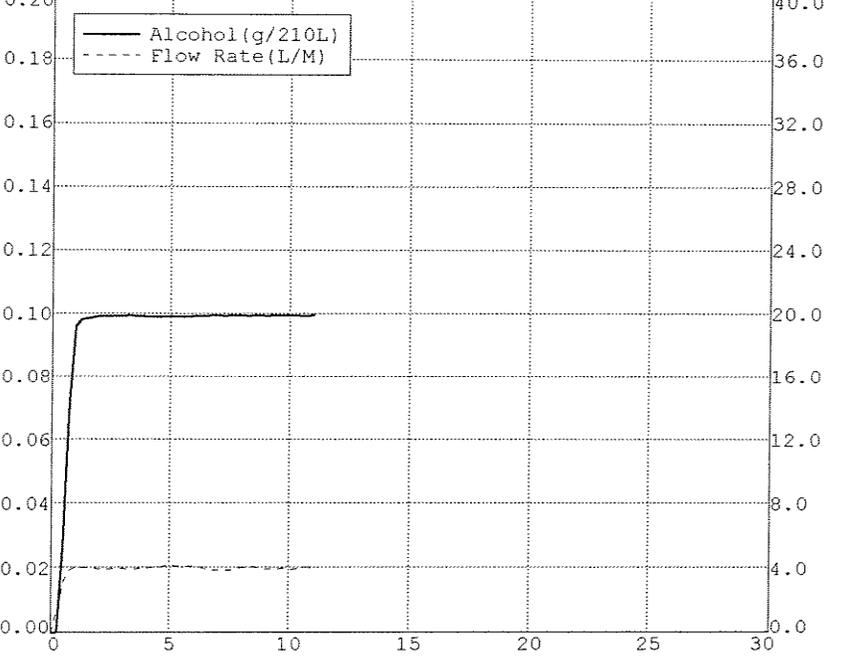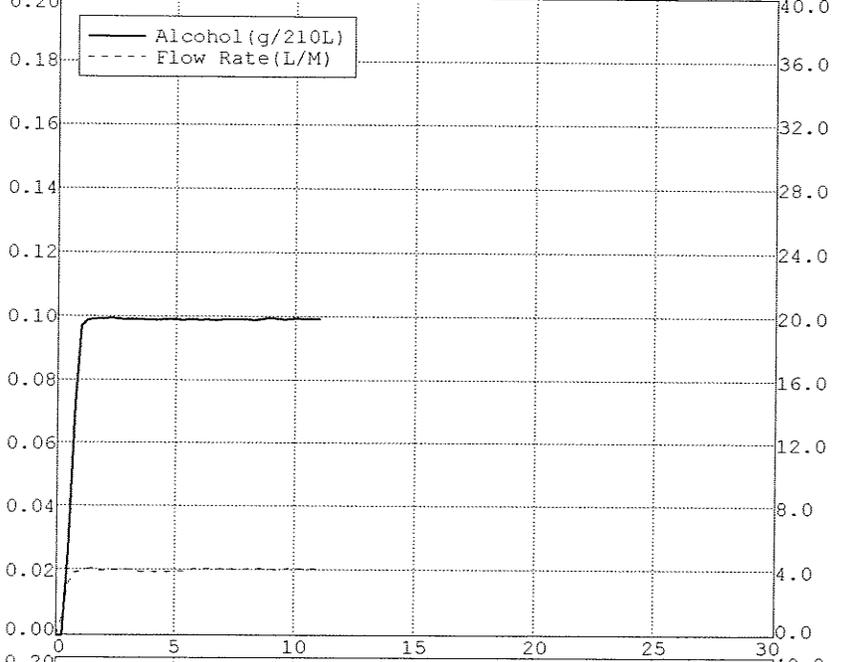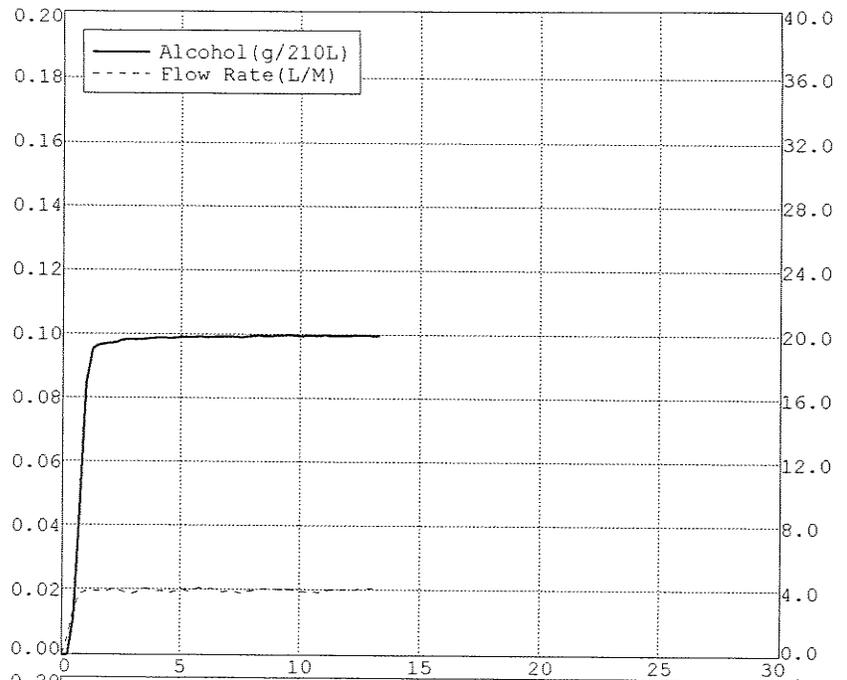

Charles B. Geisler #241