

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 12/26/2018

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:04
INTERNAL STANDARD	VERIFIED	04:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:05
BLANK TEST	0.00	04:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:06
BLANK TEST	0.00	04:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:07
BLANK TEST	0.00	04:08

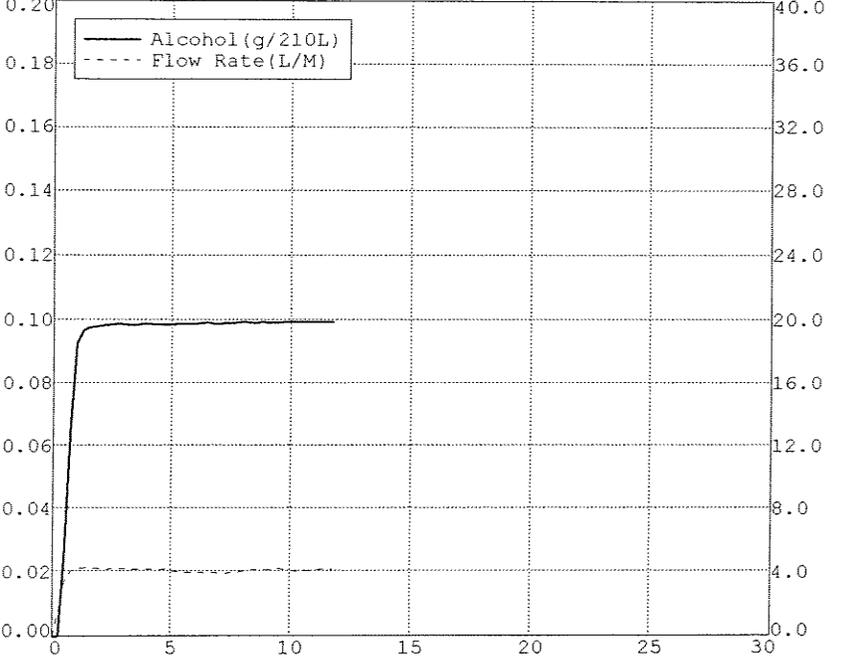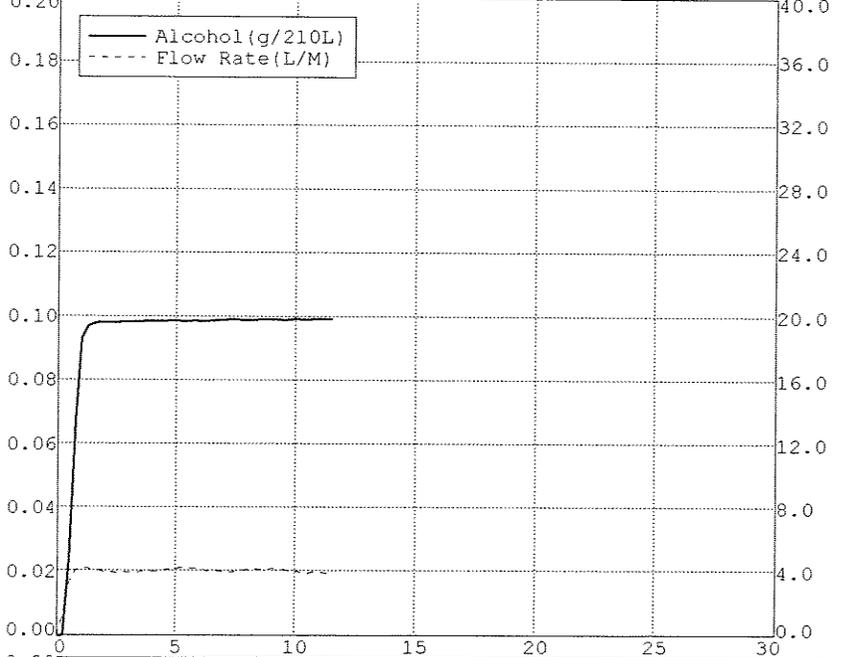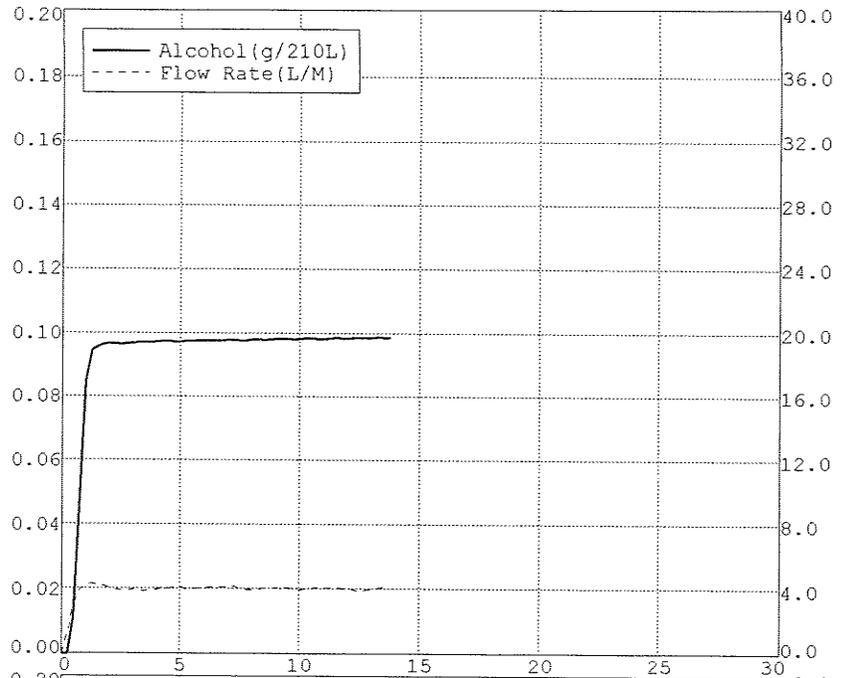

Charles B. Geisler #244