

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/04/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:06
INTERNAL STANDARD	VERIFIED	06:06
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	06:06
BLANK TEST	0.00	06:07
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	06:07
BLANK TEST	0.00	06:08
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	06:08
BLANK TEST	0.00	06:09

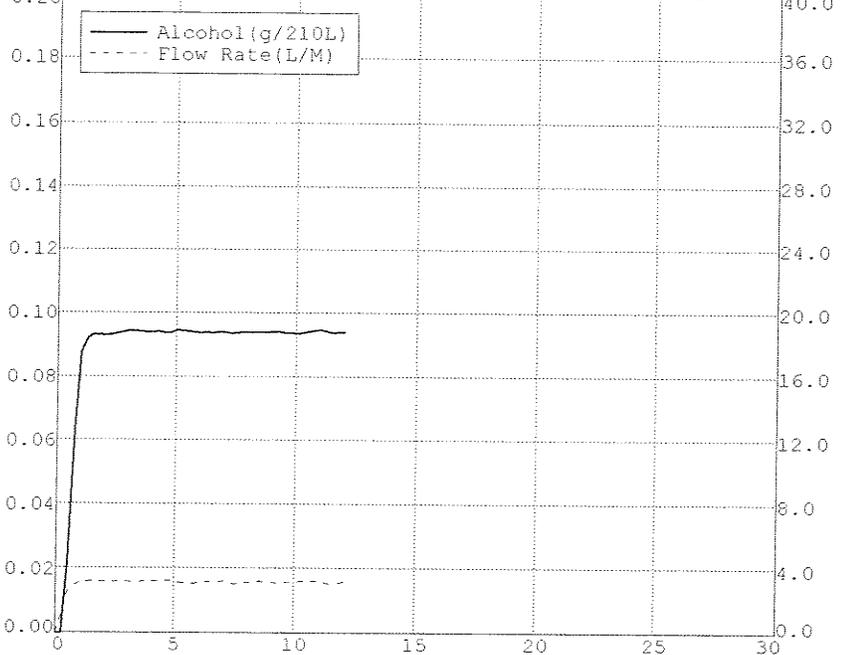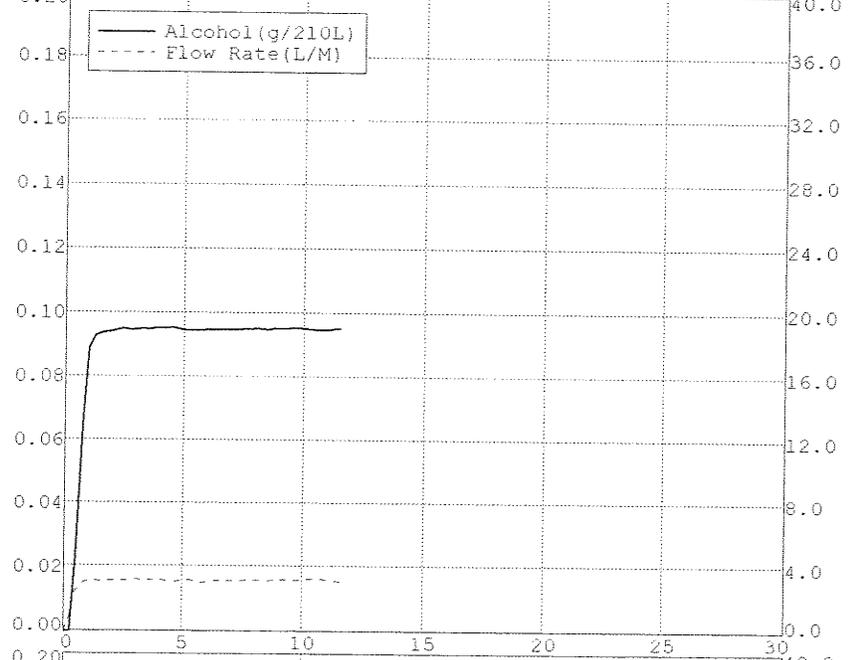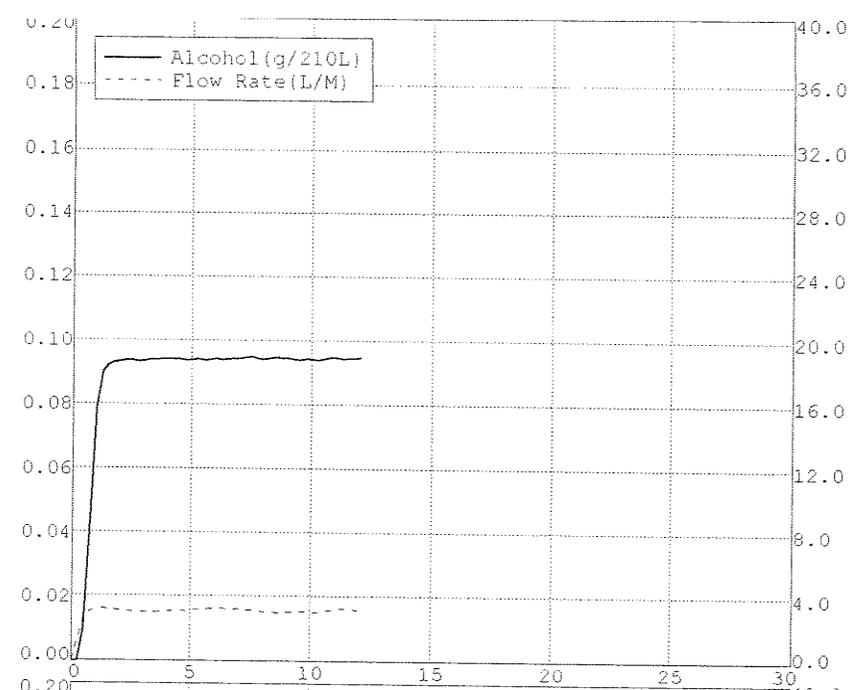

Charles B. Geisler #241