

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/13/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:25
INTERNAL STANDARD	VERIFIED	21:25
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:25
BLANK TEST	0.00	21:26
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	21:26
BLANK TEST	0.00	21:27
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	21:28
BLANK TEST	0.00	21:29

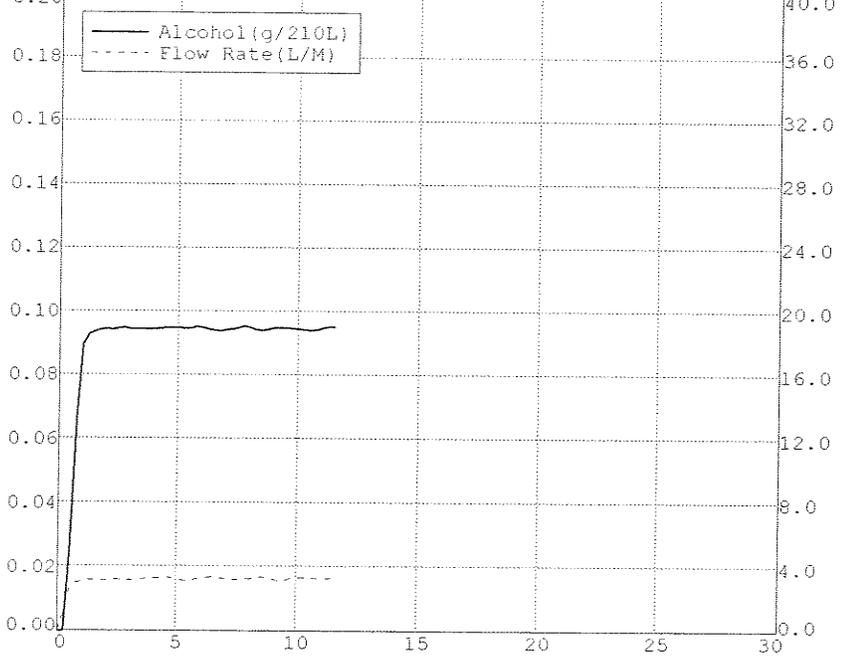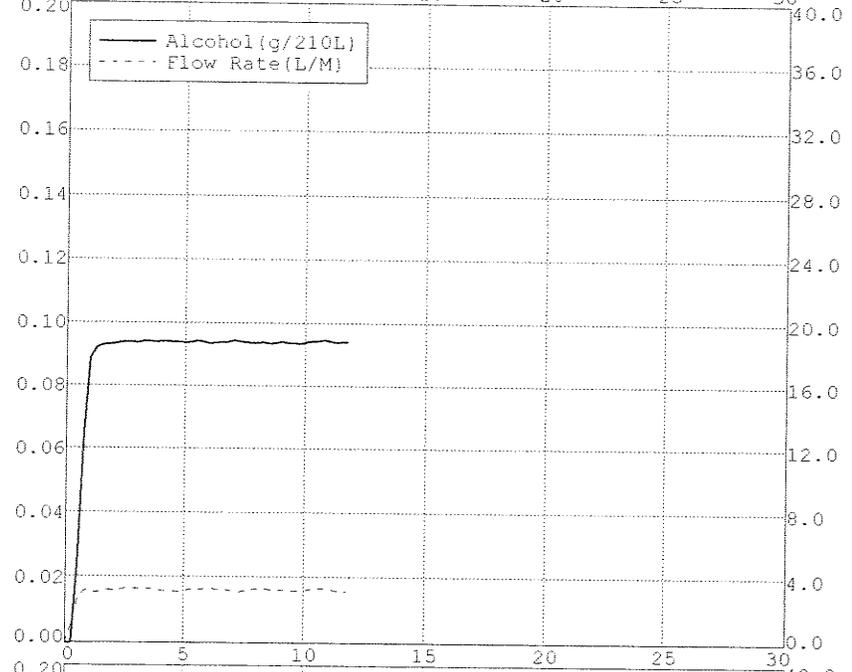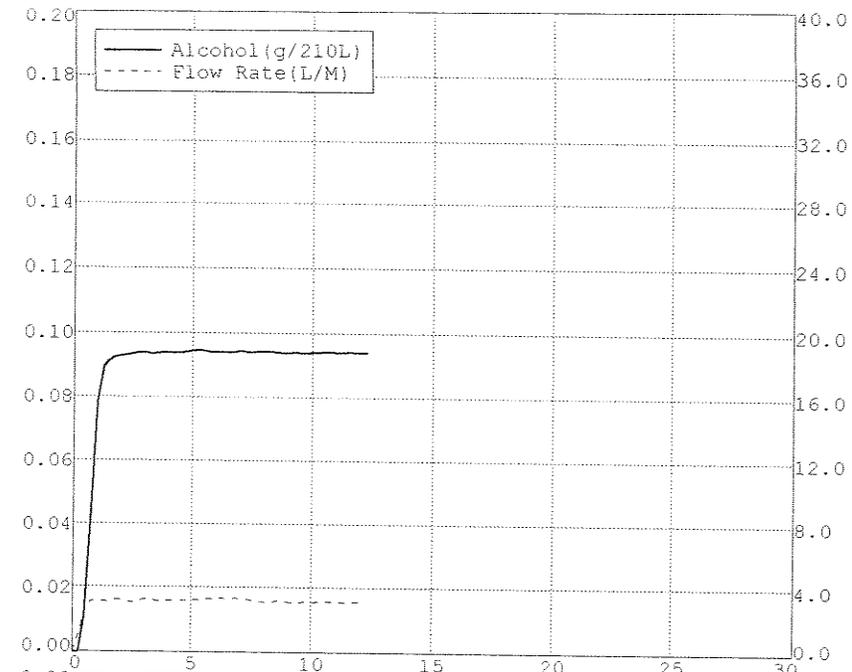

Charles B. Geisler #241