

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/19/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:36
INTERNAL STANDARD	VERIFIED	01:36
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:36
BLANK TEST	0.00	01:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:37
BLANK TEST	0.00	01:38
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:38
BLANK TEST	0.00	01:39

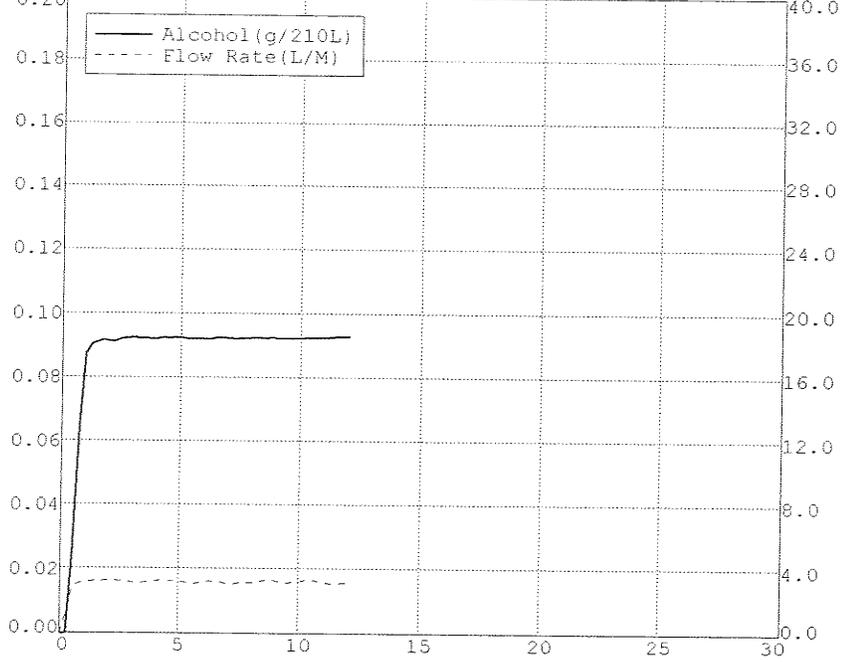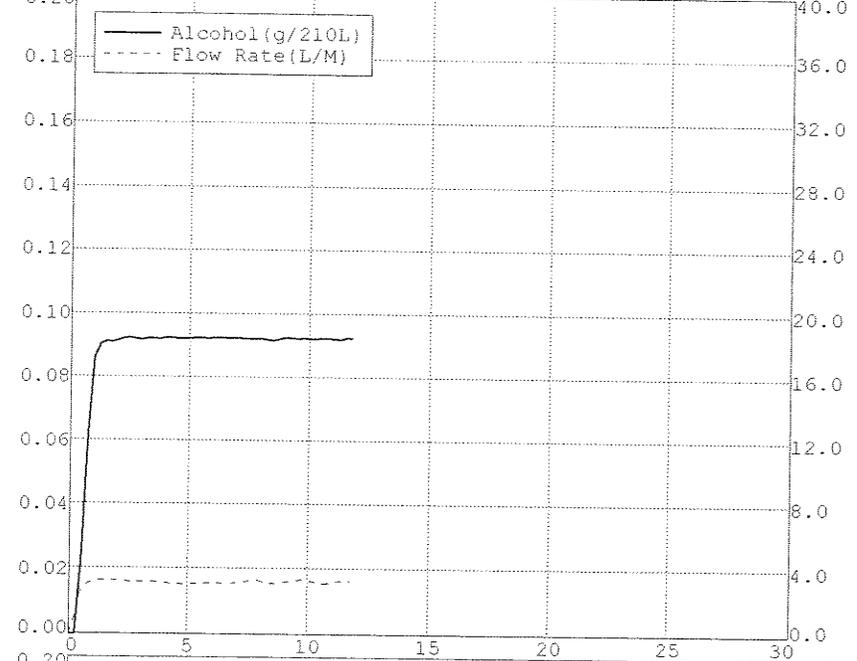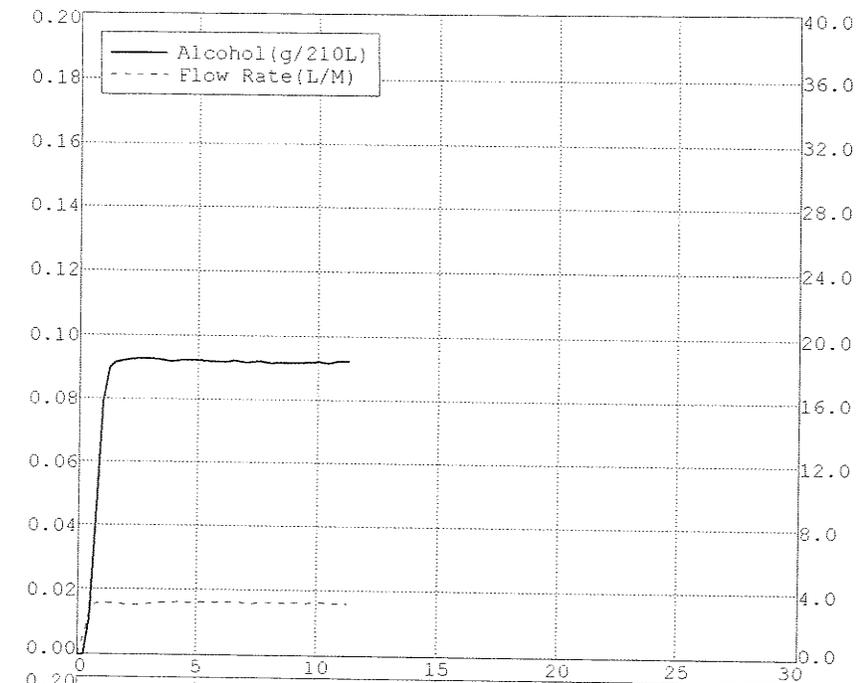

Charles B. Geisler #33757