

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 02/09/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:04
INTERNAL STANDARD	VERIFIED	22:04
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	22:04
BLANK TEST	0.00	22:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:05
BLANK TEST	0.00	22:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:06
BLANK TEST	0.00	22:07

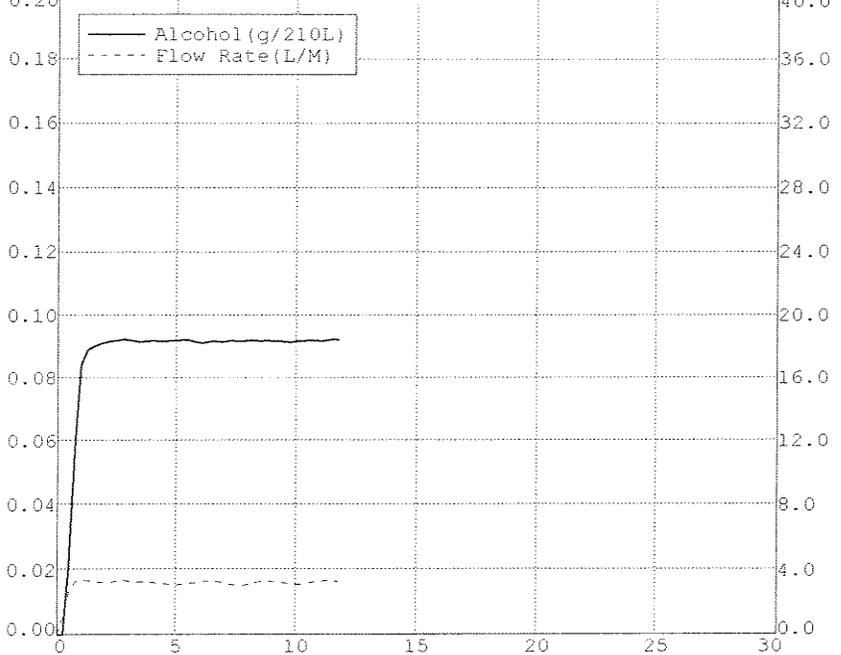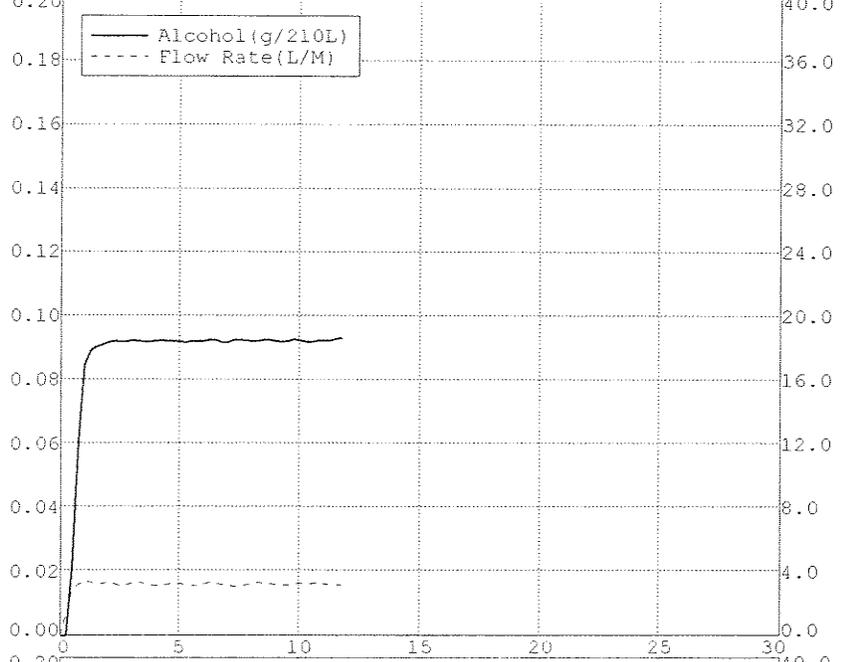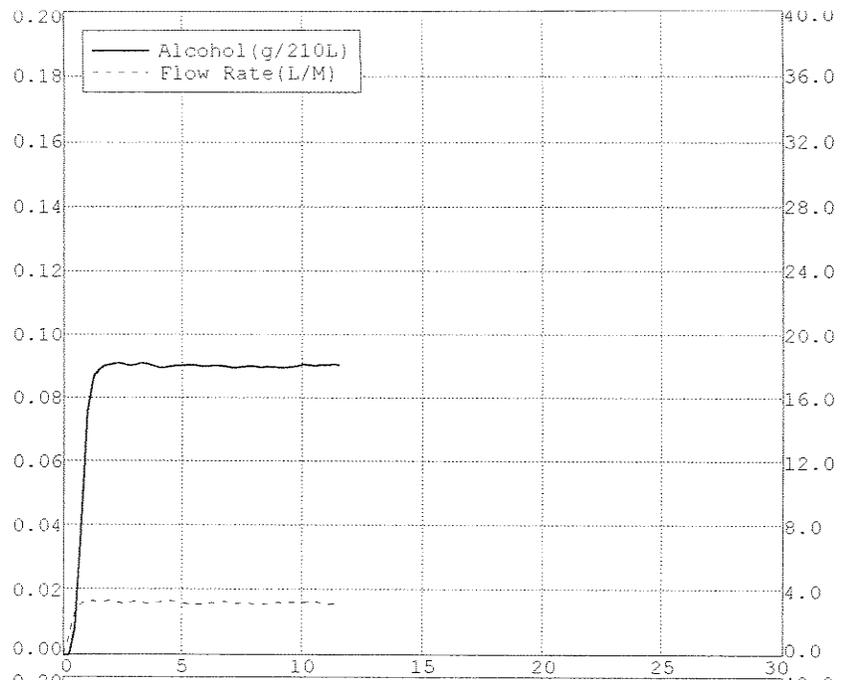

*Handwritten signature and initials*