

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/16/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:23
INTERNAL STANDARD	VERIFIED	00:23
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	00:23
BLANK TEST	0.00	00:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:24
BLANK TEST	0.00	00:25
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:26
BLANK TEST	0.00	00:27

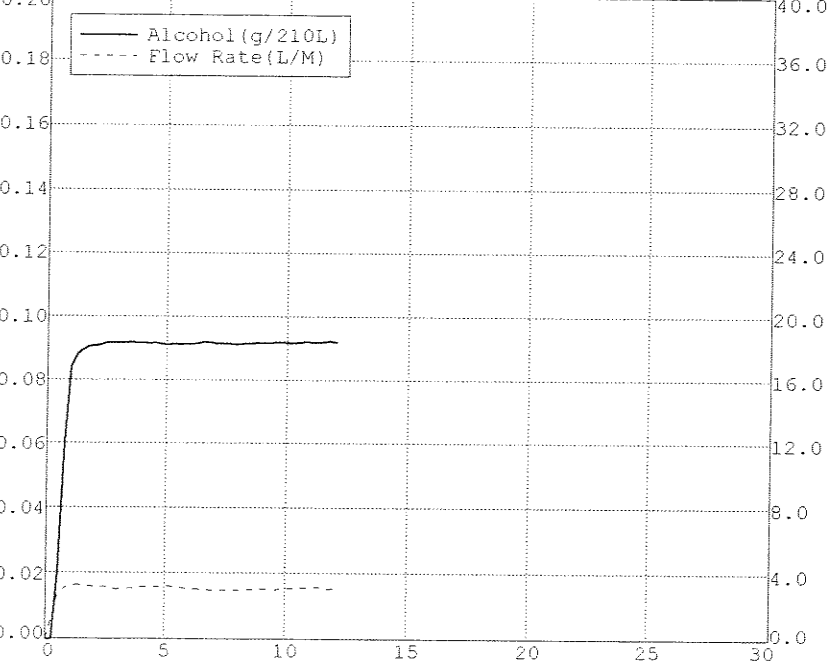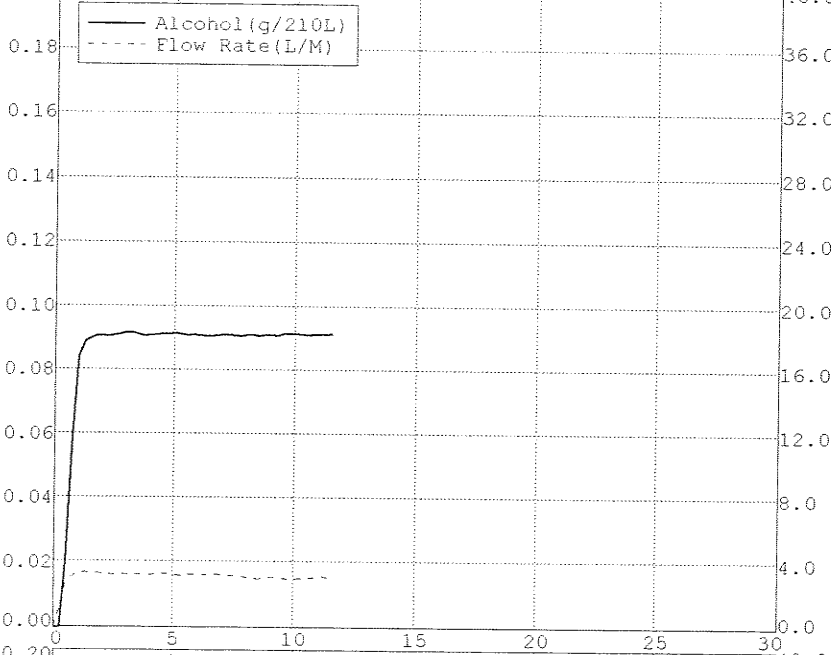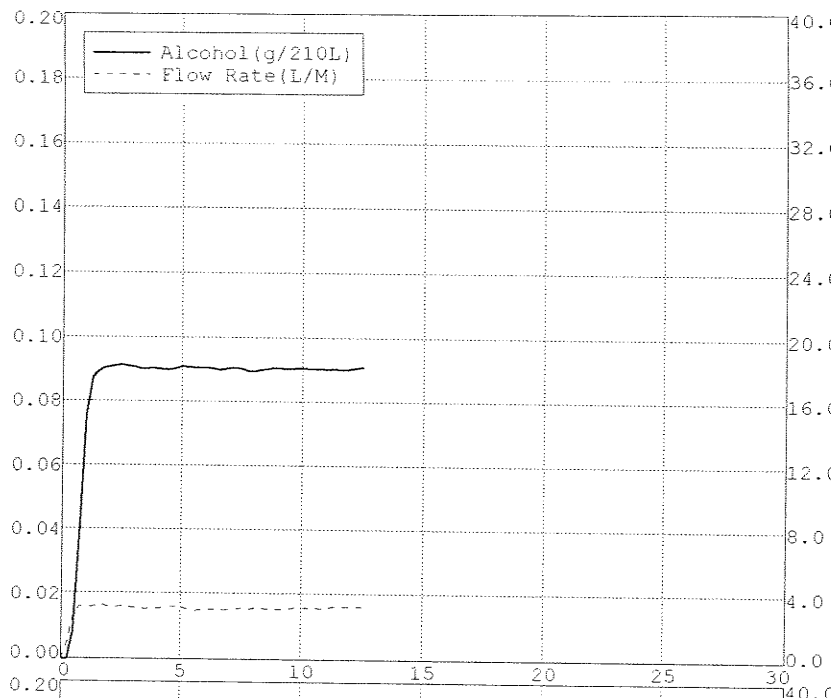

Signature: Charles B. Geisler #246