

SOLUTION CHANGE




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606

Date: 03/01/2018

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:46
INTERNAL STANDARD	VERIFIED	04:46
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	04:47
BLANK TEST	0.00	04:48
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	04:48
BLANK TEST	0.00	04:49
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	04:49
BLANK TEST	0.00	04:50

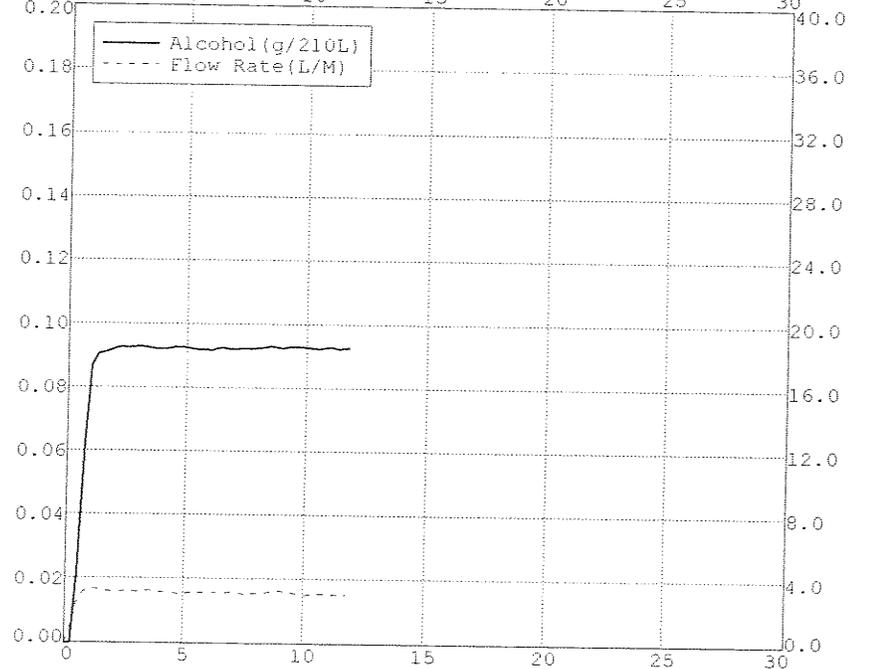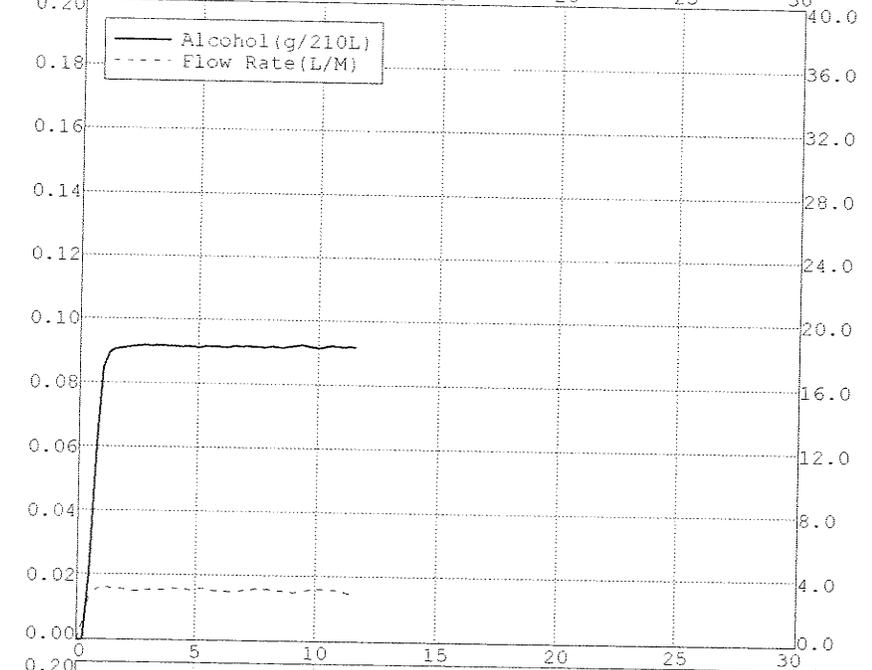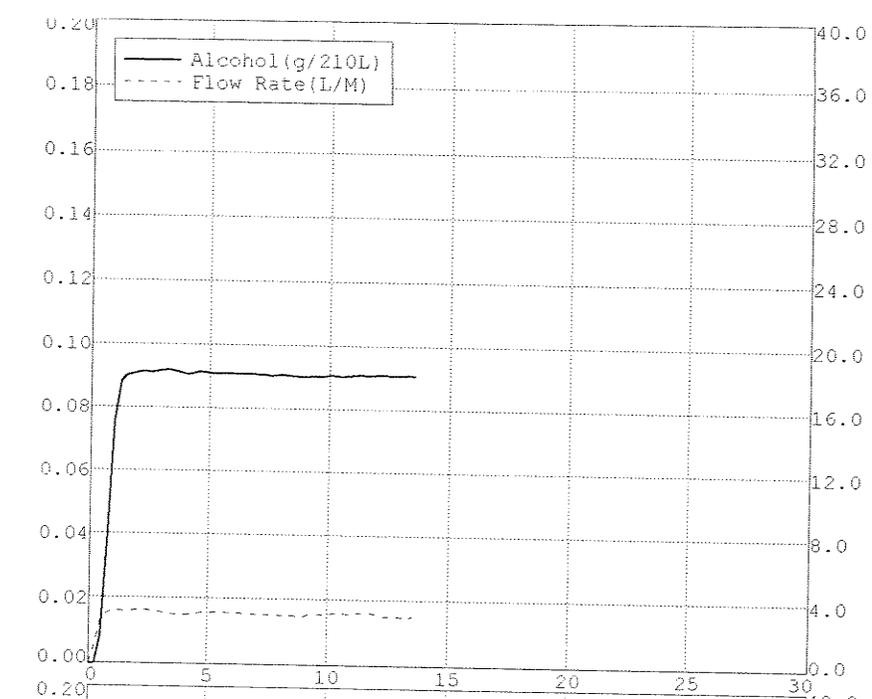

*Charles B Geisler*