

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 03/07/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:21
INTERNAL STANDARD	VERIFIED	02:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:21
BLANK TEST	0.00	02:22
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	02:22
BLANK TEST	0.00	02:23
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:24
BLANK TEST	0.00	02:24

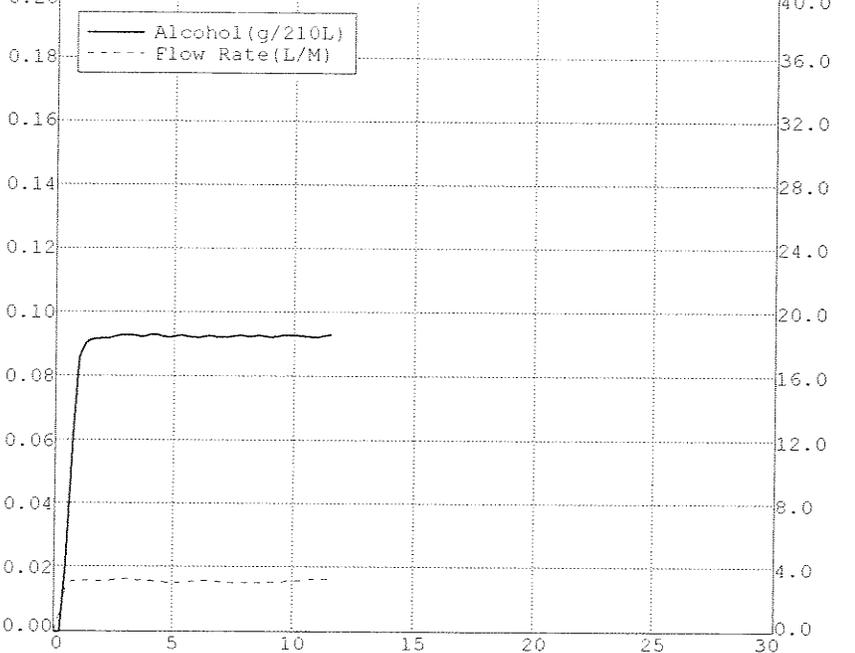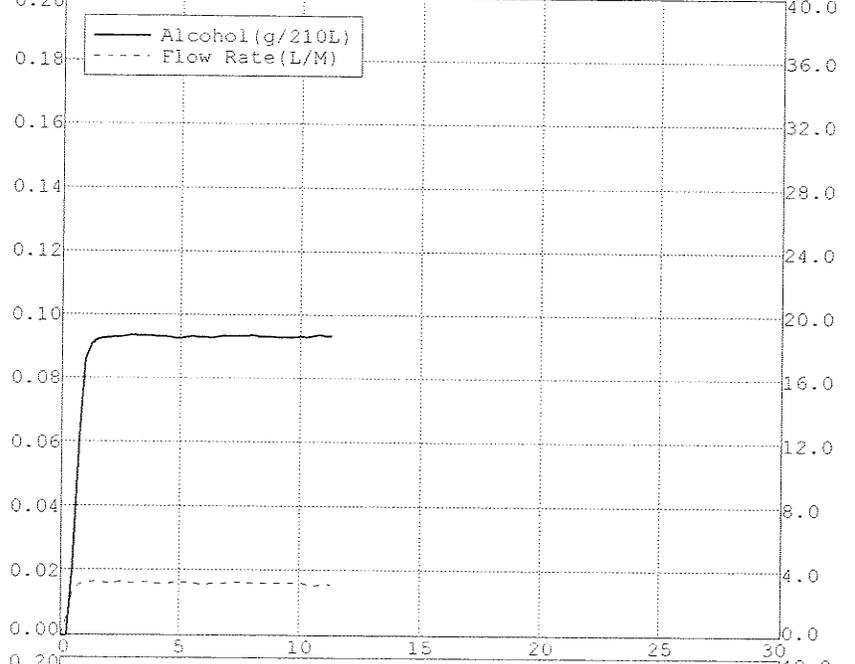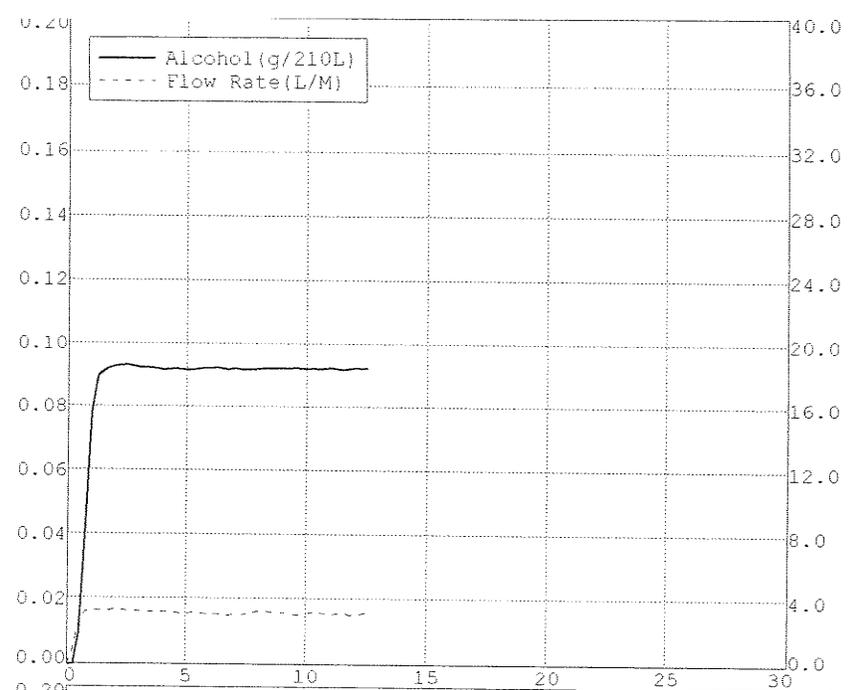

*Charles B Geisler* #241