

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 03/24/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:24
INTERNAL STANDARD	VERIFIED	00:24
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:24
BLANK TEST	0.00	00:25
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:25
BLANK TEST	0.00	00:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:27
BLANK TEST	0.00	00:28

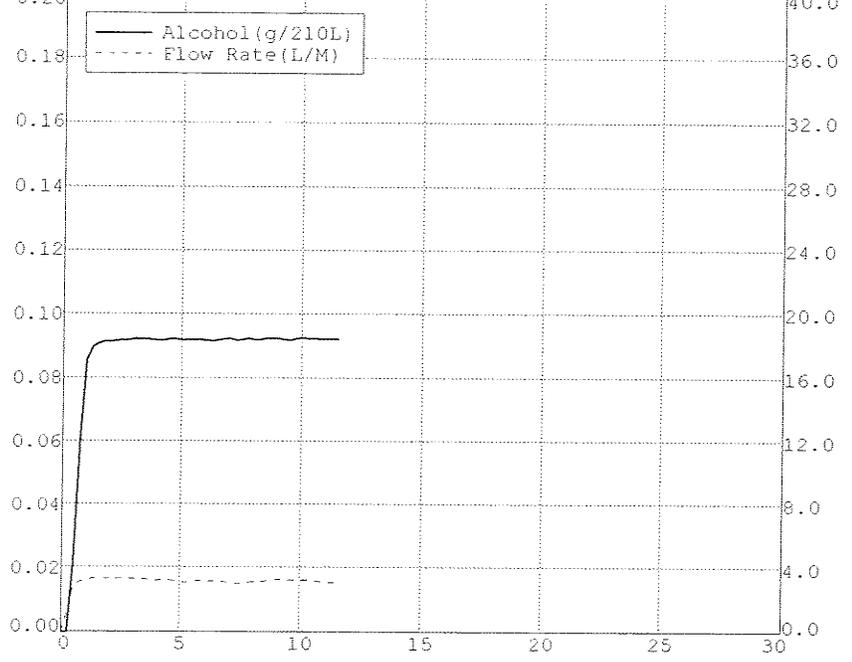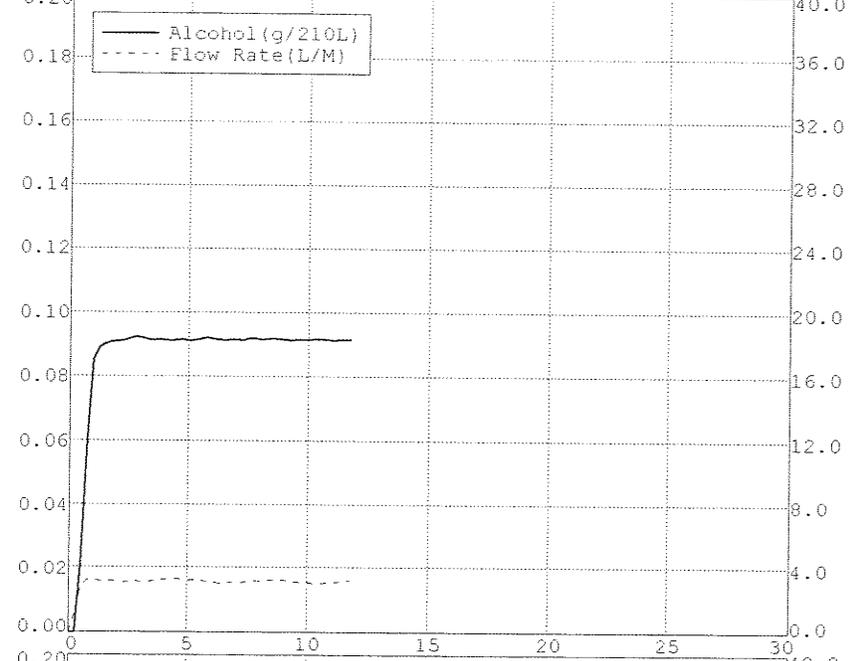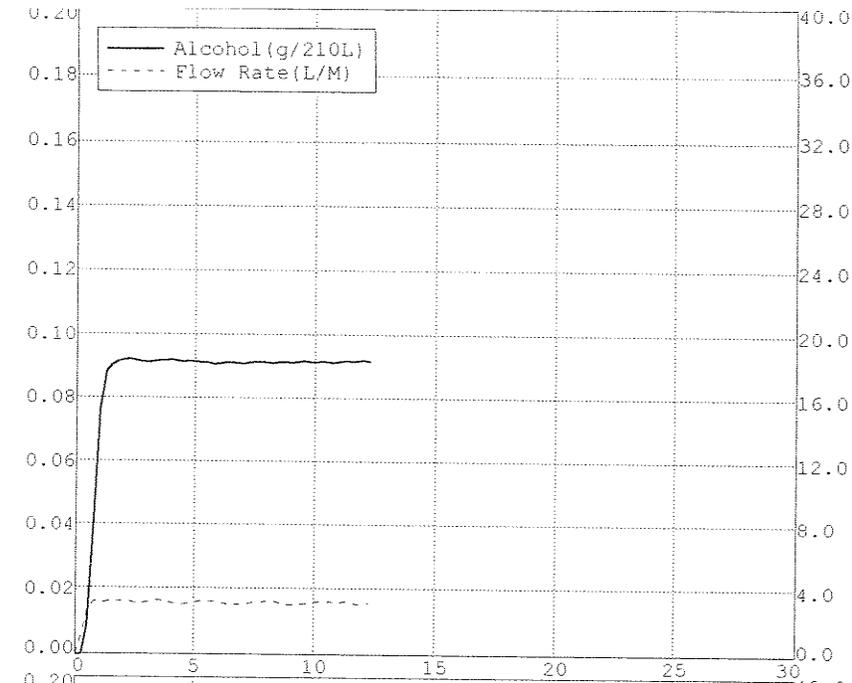

Charles B Geisler #241