

SOLUTION CHANGE




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 03/30/2018

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:48
INTERNAL STANDARD	VERIFIED	03:48
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	03:48
BLANK TEST	0.00	03:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:50
BLANK TEST	0.00	03:50
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	03:51
BLANK TEST	0.00	03:52

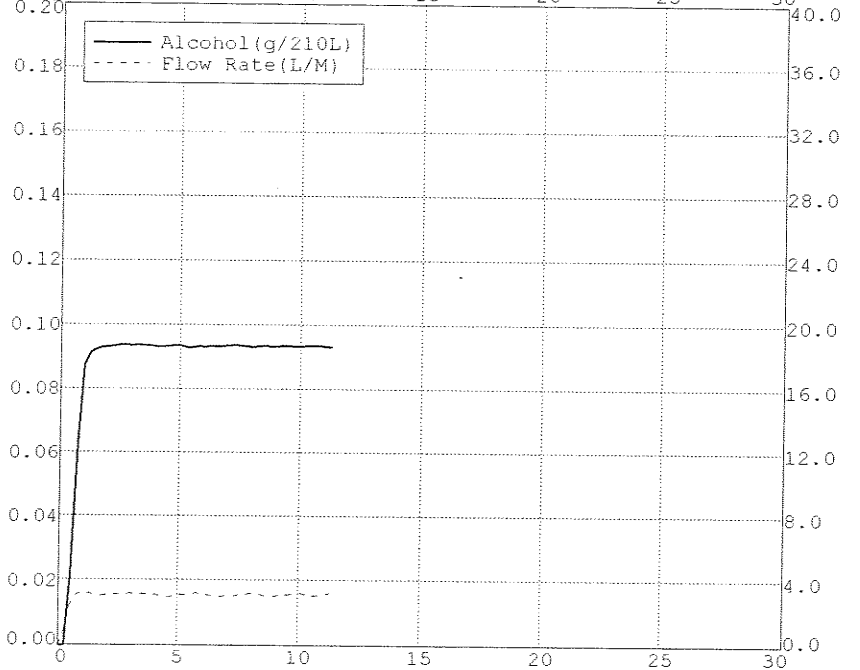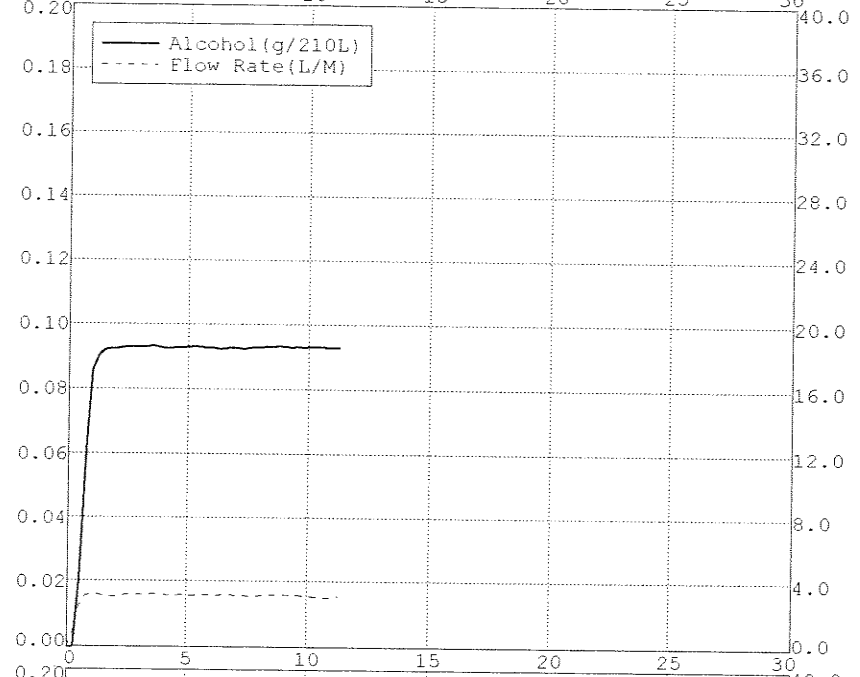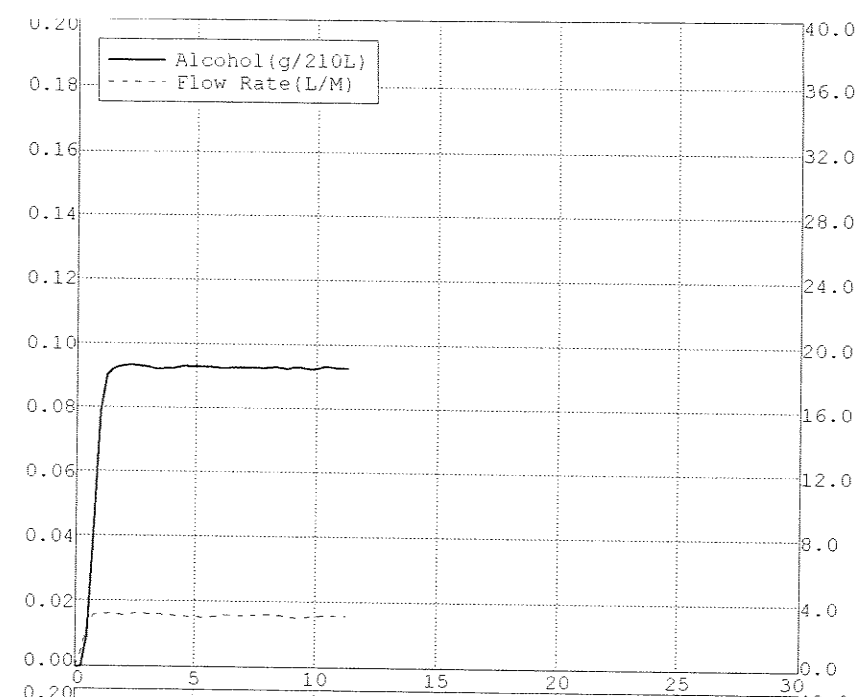

Charles B. Geisler