

SUPERVISOR TEST


WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 04/06/2018

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:10
INTERNAL STANDARD	VERIFIED	22:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	22:11
BLANK TEST	0.00	22:11
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	22:12
BLANK TEST	0.00	22:13
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	22:13
BLANK TEST	0.00	22:14

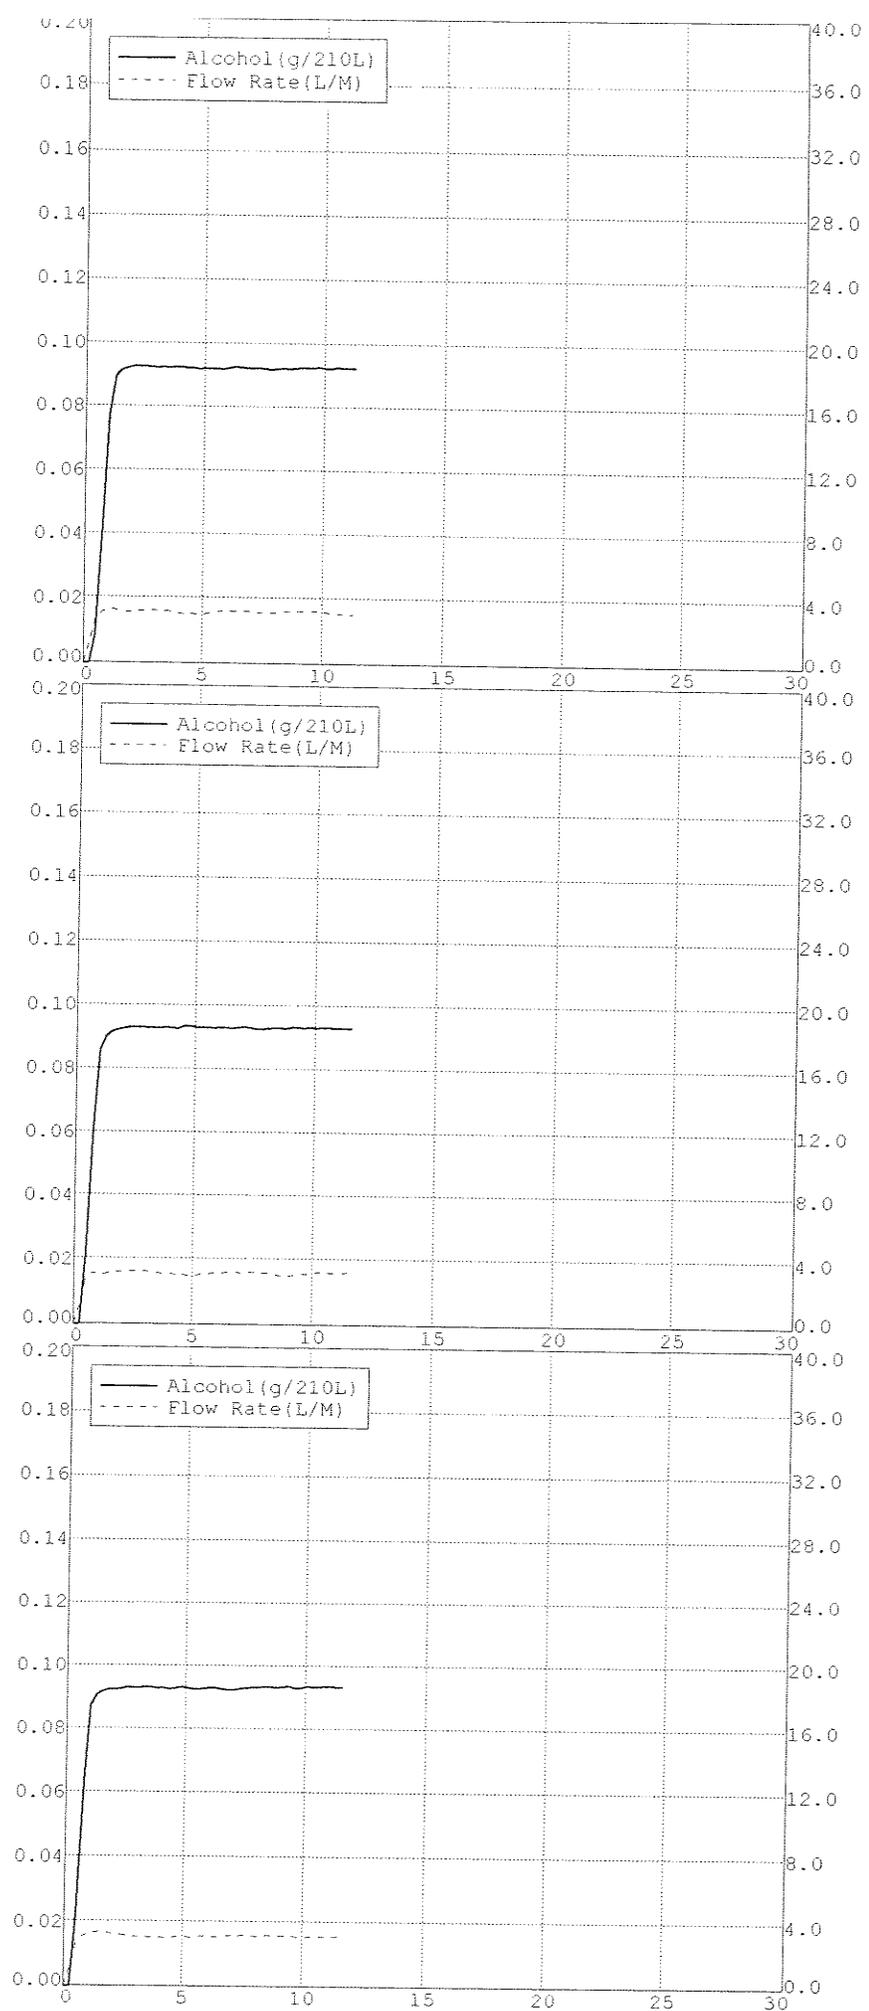

Charles B. Geisler #241