

SOLUTION CHANGE




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606

Date: 05/02/2018

OPERATOR NAME:  
 RYAN C SCHROECK  
 Permit #: 41316  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:22
INTERNAL STANDARD	VERIFIED	09:22
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	09:23
BLANK TEST	0.00	09:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:24
BLANK TEST	0.00	09:25
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	09:25
BLANK TEST	0.00	09:26

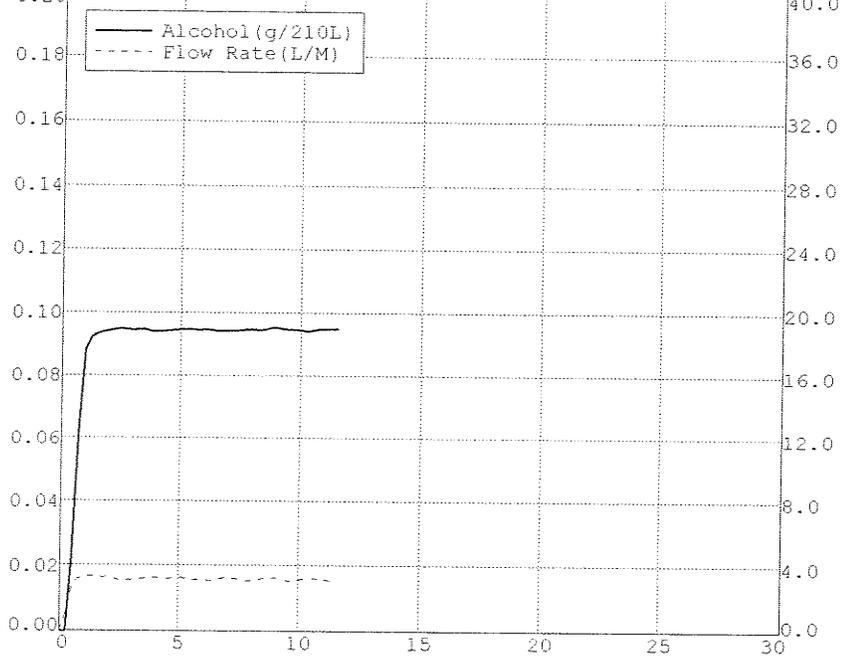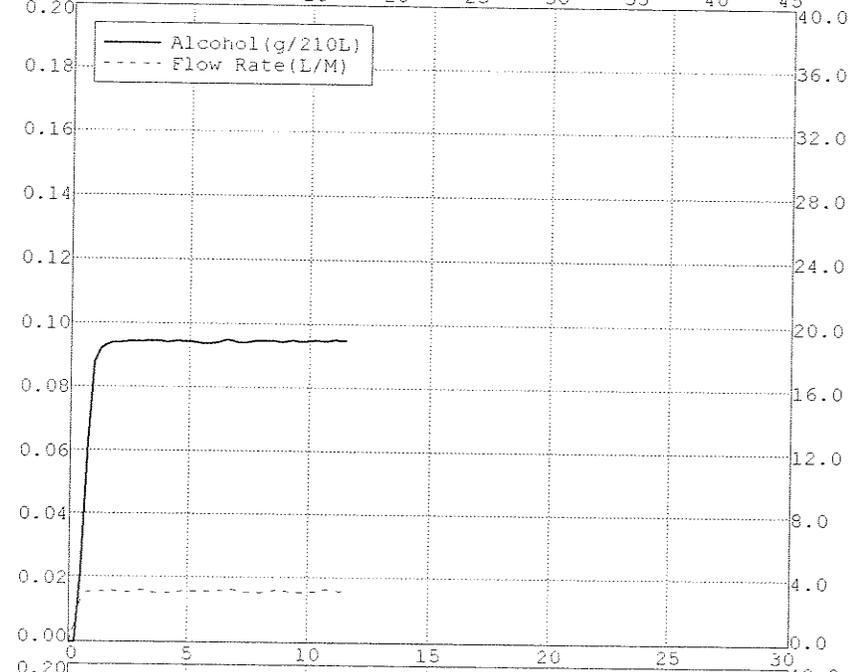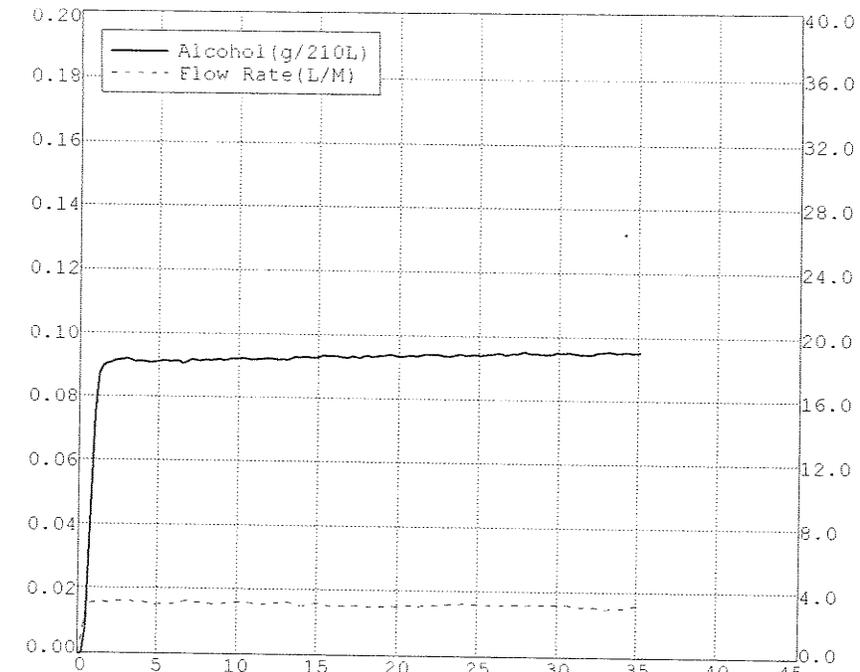

*Handwritten signature and number: Ryan C Schroeck 724*