

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 05/08/2018

OPERATOR NAME:  
J T COON  
Permit #: 36043  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:43
INTERNAL STANDARD	VERIFIED	19:44
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	19:44
BLANK TEST	0.00	19:45
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	19:45
BLANK TEST	0.00	19:46
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	19:46
BLANK TEST	0.00	19:47

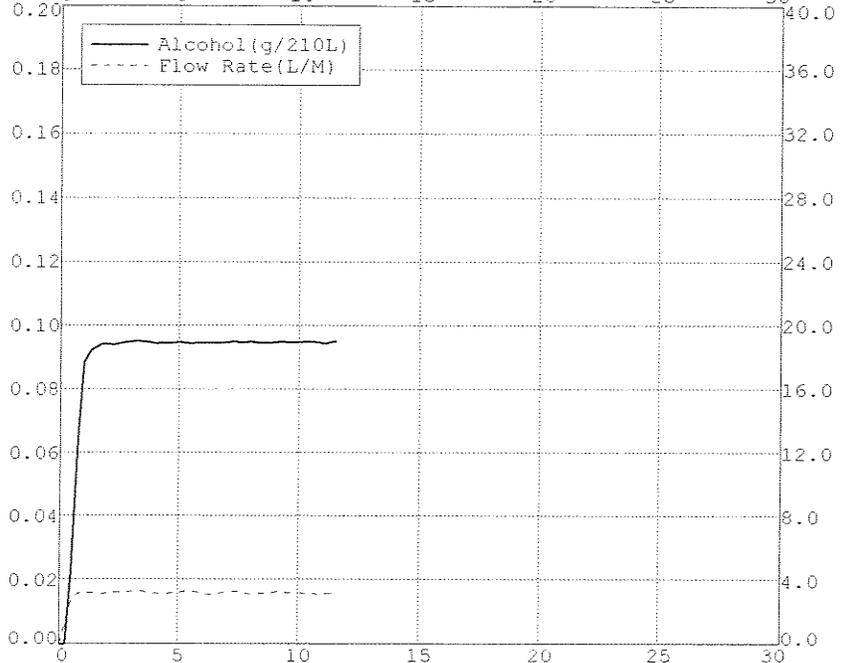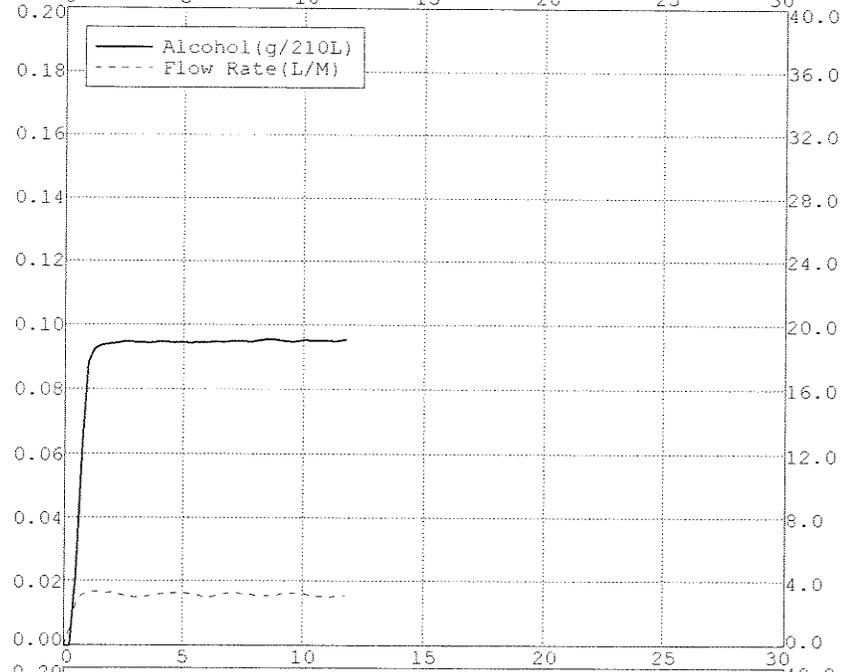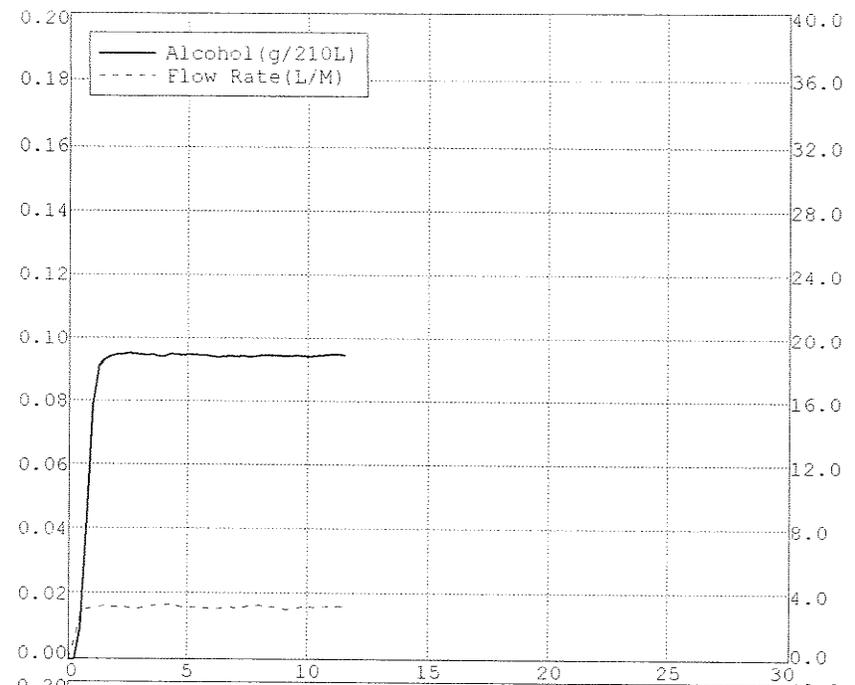

*J T Coon* 341