

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 05/15/2018

OPERATOR NAME:
TYLER J MORSE
Permit #: 41959
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:53
INTERNAL STANDARD	VERIFIED	13:53
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	13:54
BLANK TEST	0.00	13:55
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	13:55
BLANK TEST	0.00	13:56
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	13:56
BLANK TEST	0.00	13:57

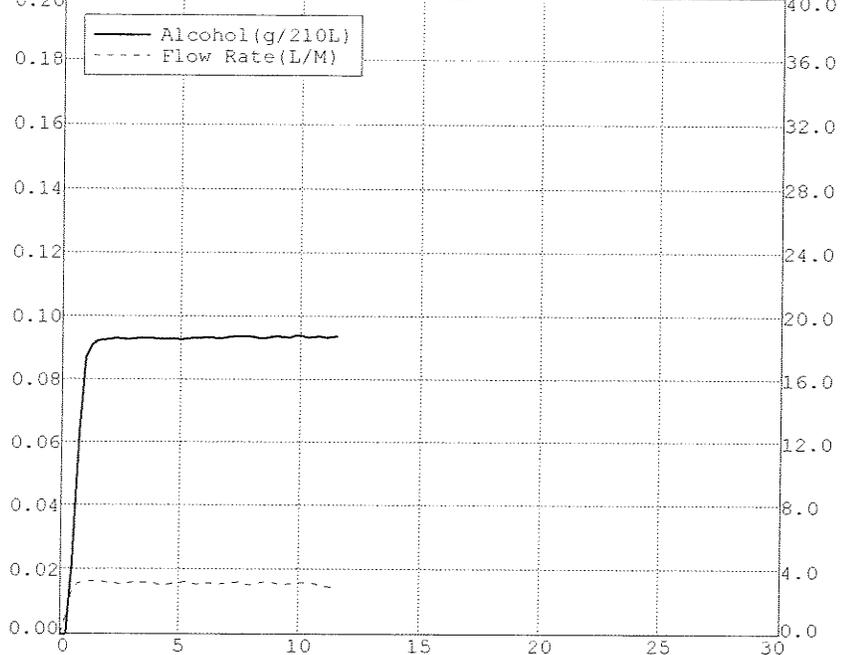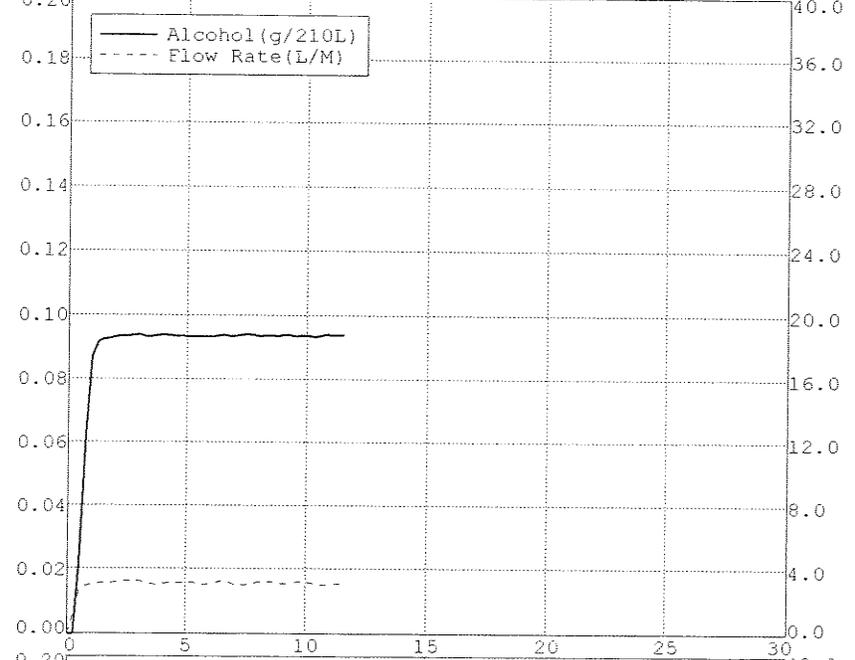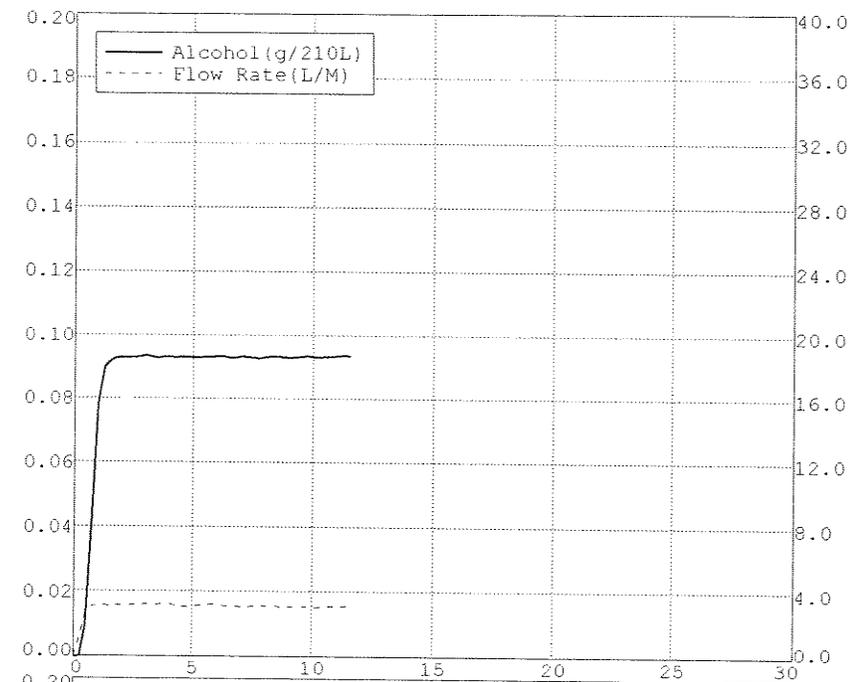

POD #447