

SOLUTION CHANGE




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 06/01/2018

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:15
INTERNAL STANDARD	VERIFIED	22:15
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	22:15
BLANK TEST	0.00	22:16
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	22:16
BLANK TEST	0.00	22:17
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	22:17
BLANK TEST	0.00	22:18

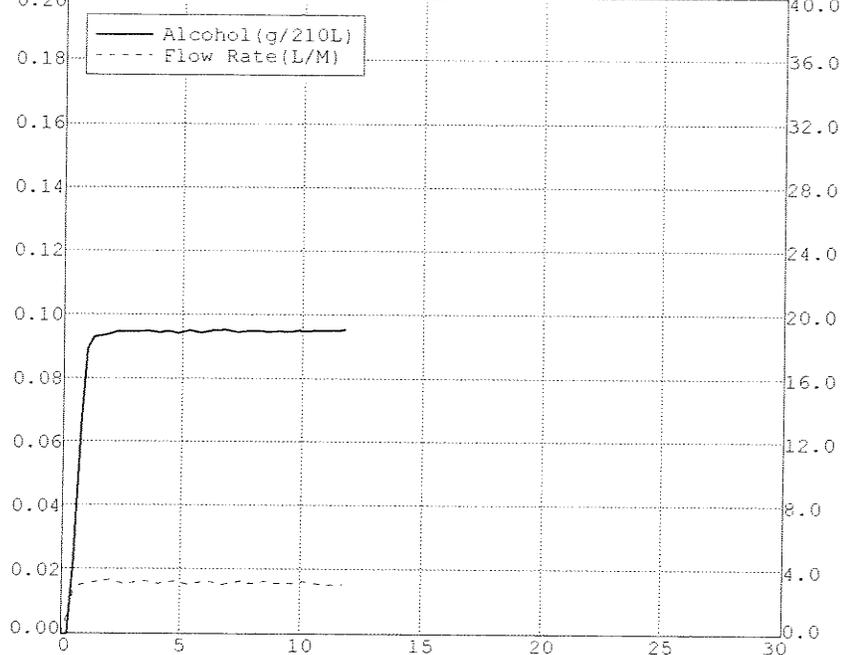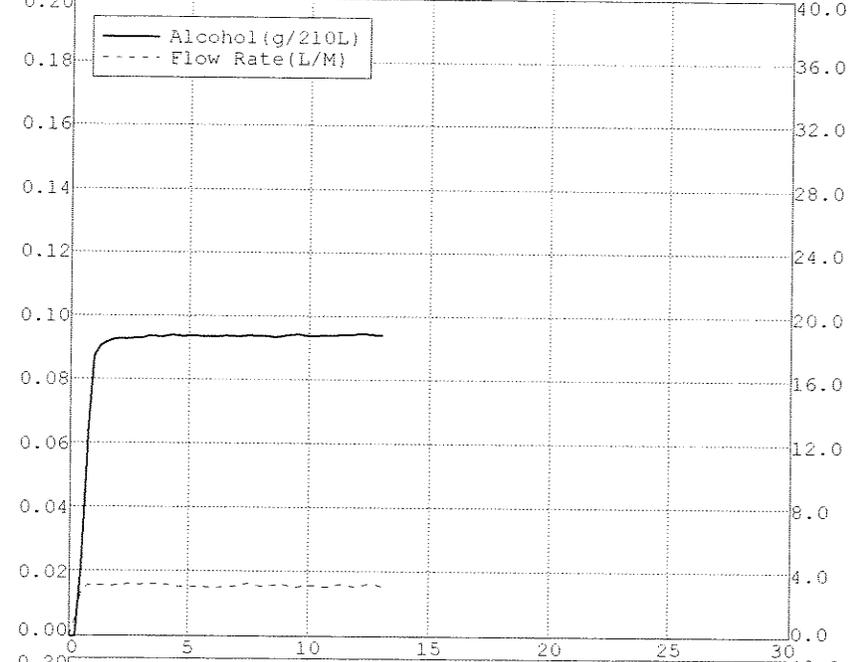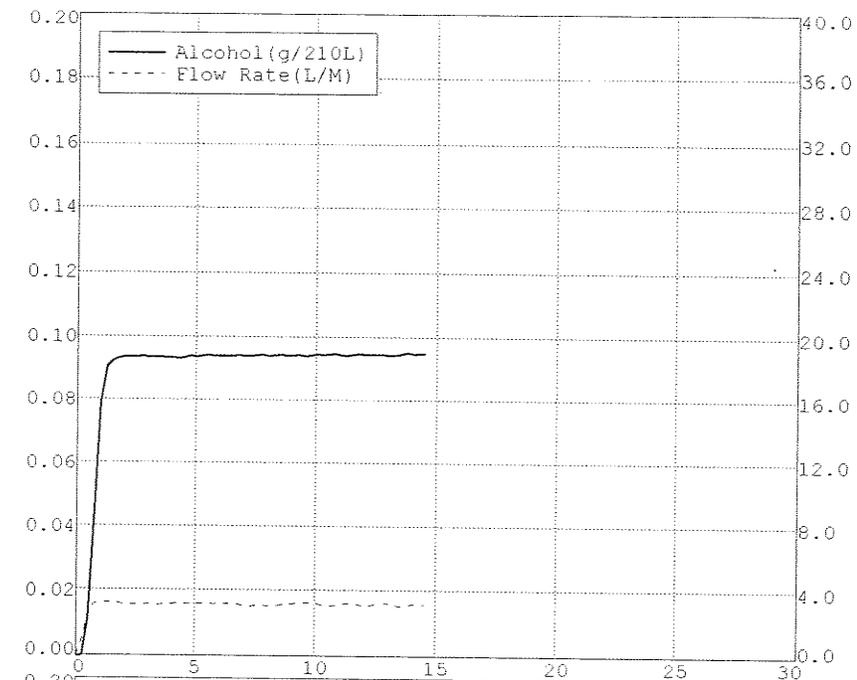

Charles B. Geisler #241