

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 06/21/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:56
INTERNAL STANDARD	VERIFIED	21:56
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:56
BLANK TEST	0.00	21:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:57
BLANK TEST	0.00	21:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:59
BLANK TEST	0.00	22:00

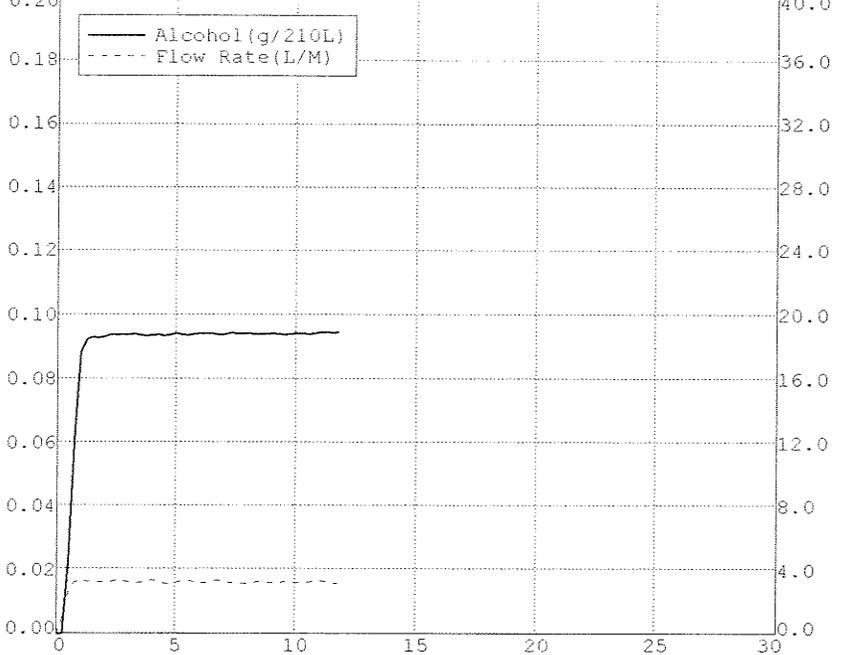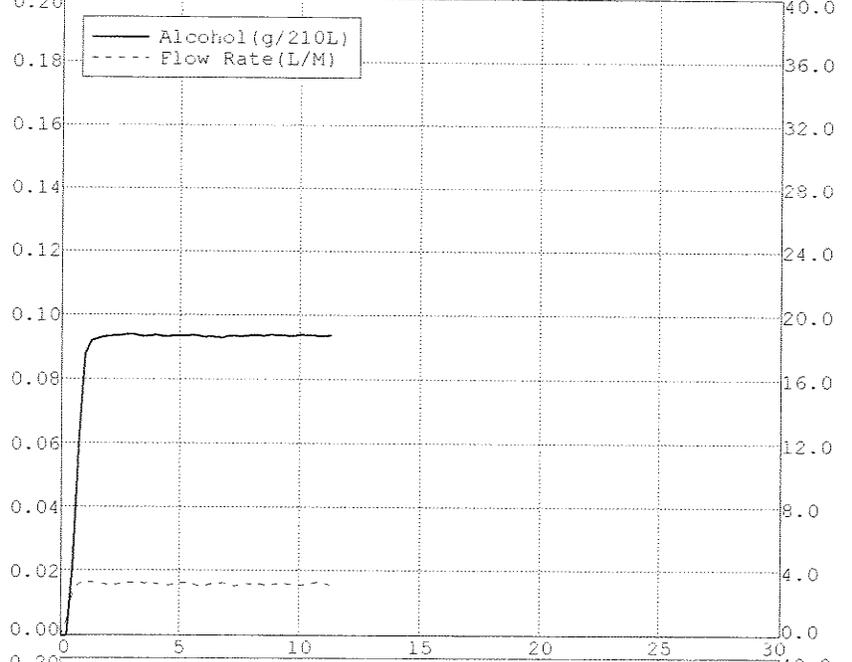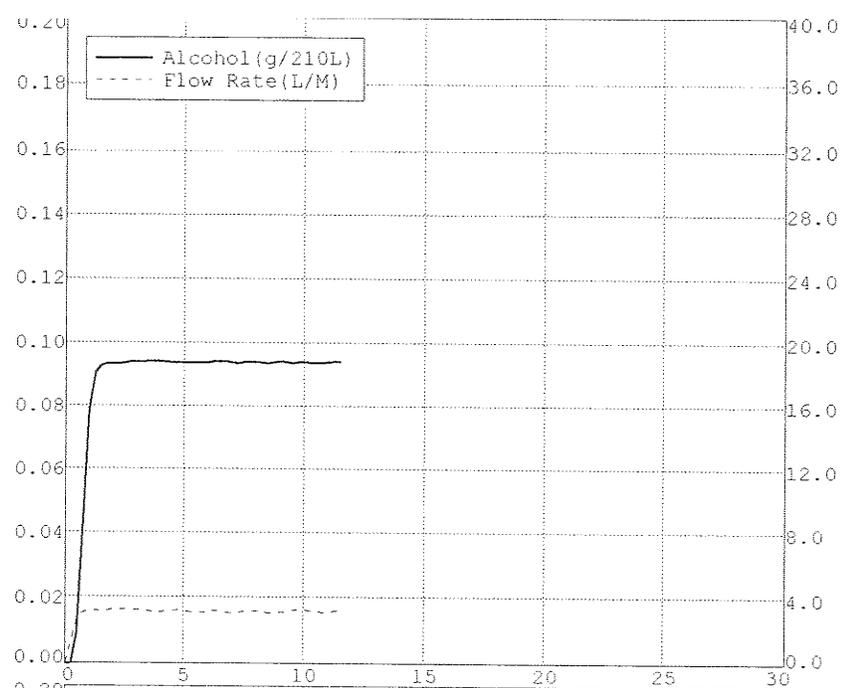

Charles B. Geisler #24