

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 06/29/2018

OPERATOR NAME:  
RYAN C SCHROECK  
Permit #: 41316  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:09
INTERNAL STANDARD	VERIFIED	08:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:09
BLANK TEST	0.00	08:10
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	08:10
BLANK TEST	0.00	08:11
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:12
BLANK TEST	0.00	08:12

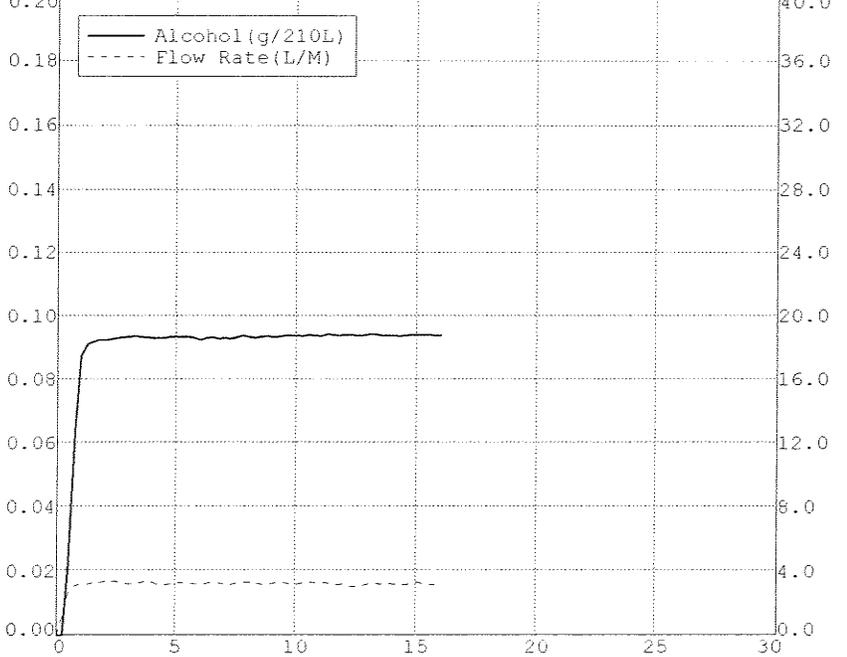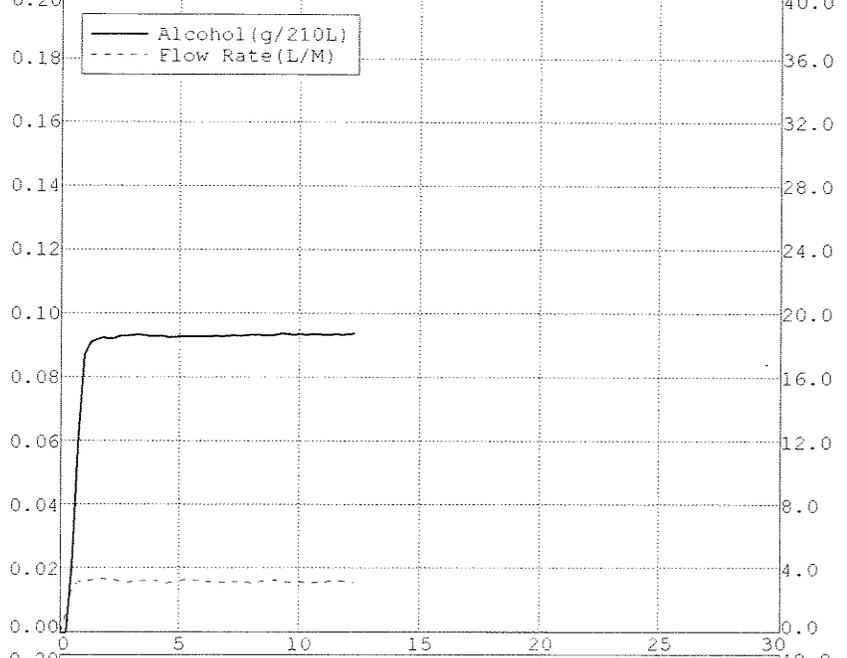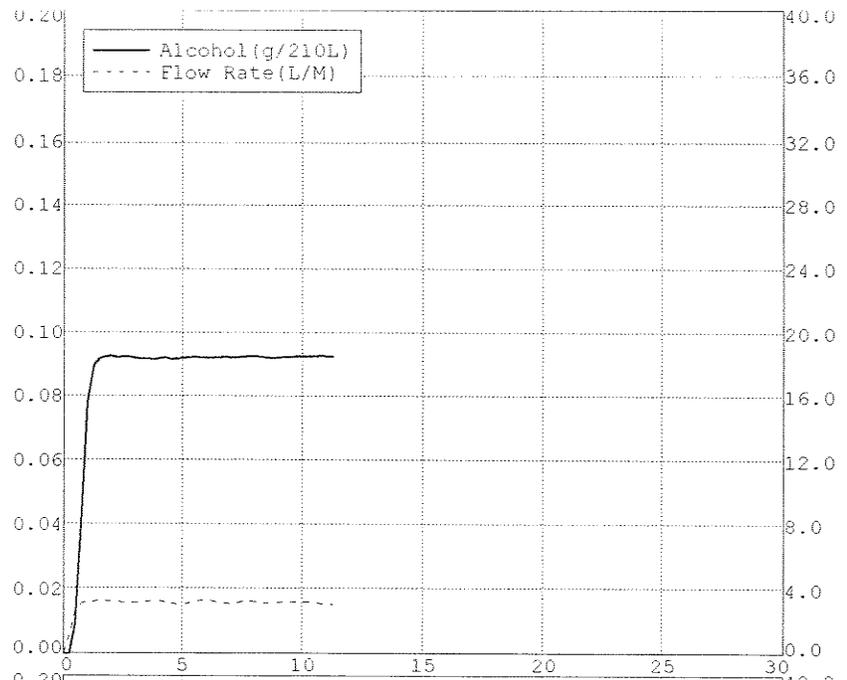

*Handwritten signature*