

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 07/15/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:44
INTERNAL STANDARD	VERIFIED	02:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:45
BLANK TEST	0.00	02:46
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:46
BLANK TEST	0.00	02:47
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	02:47
BLANK TEST	0.00	02:48

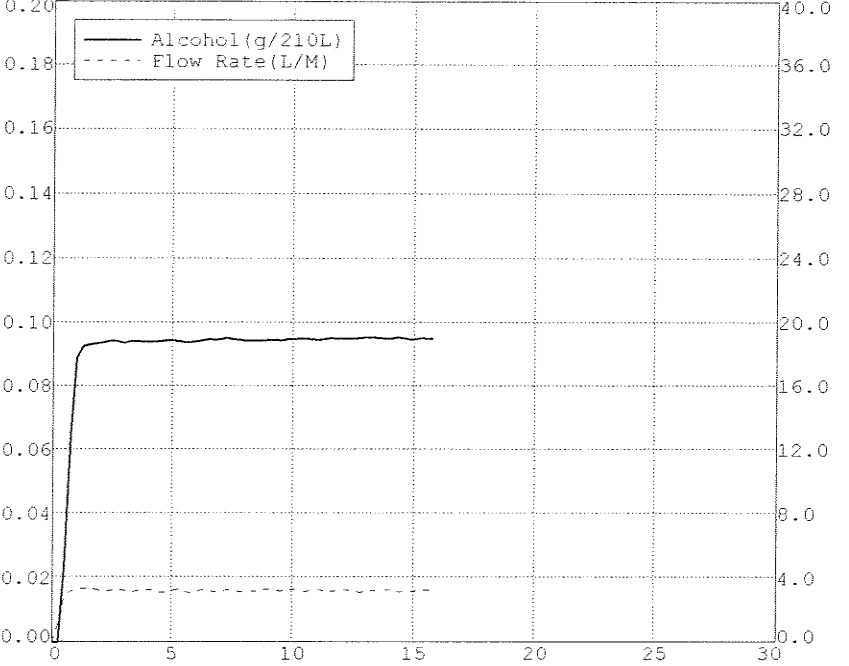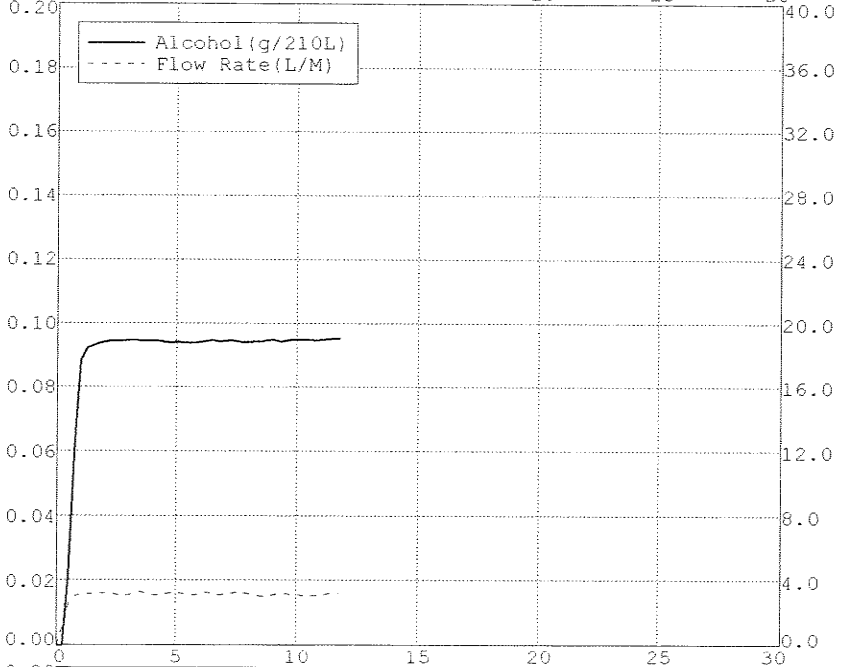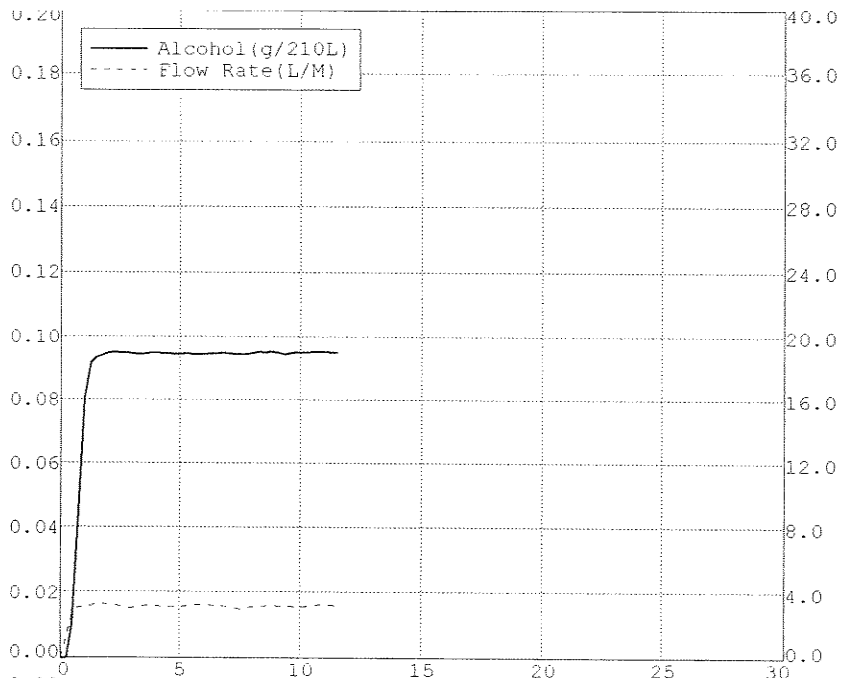

Charles B Geisler #201