

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 07/23/2018

OPERATOR NAME:  
RYAN C SCHROECK  
Permit #: 41316  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:49
INTERNAL STANDARD	VERIFIED	15:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	15:50
BLANK TEST	0.00	15:51
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	15:51
BLANK TEST	0.00	15:52
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	15:52
BLANK TEST	0.00	15:53

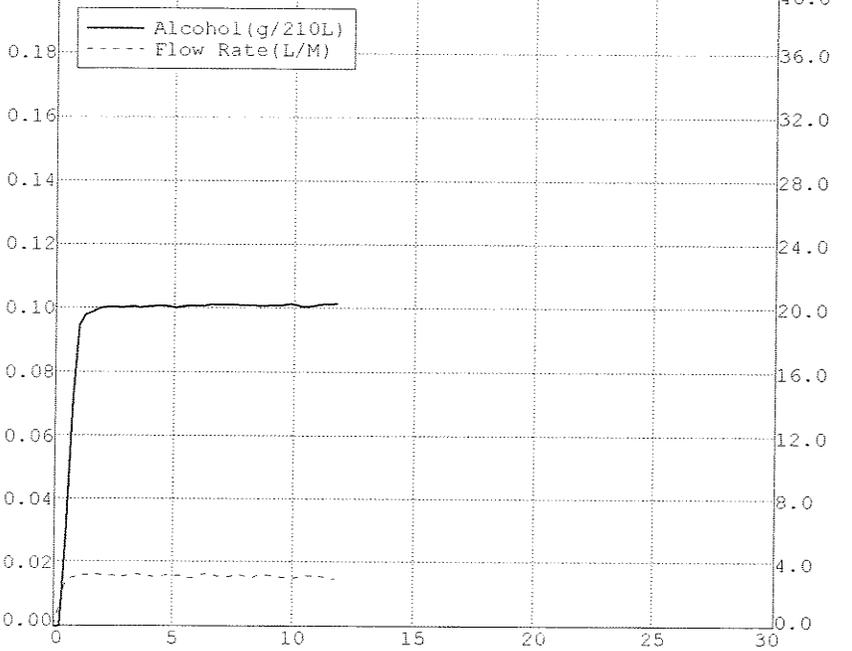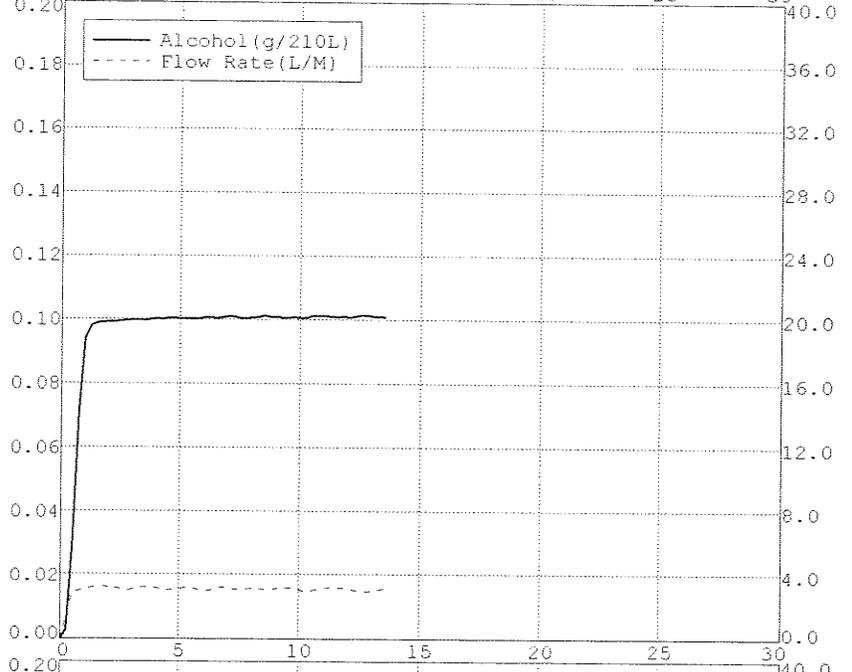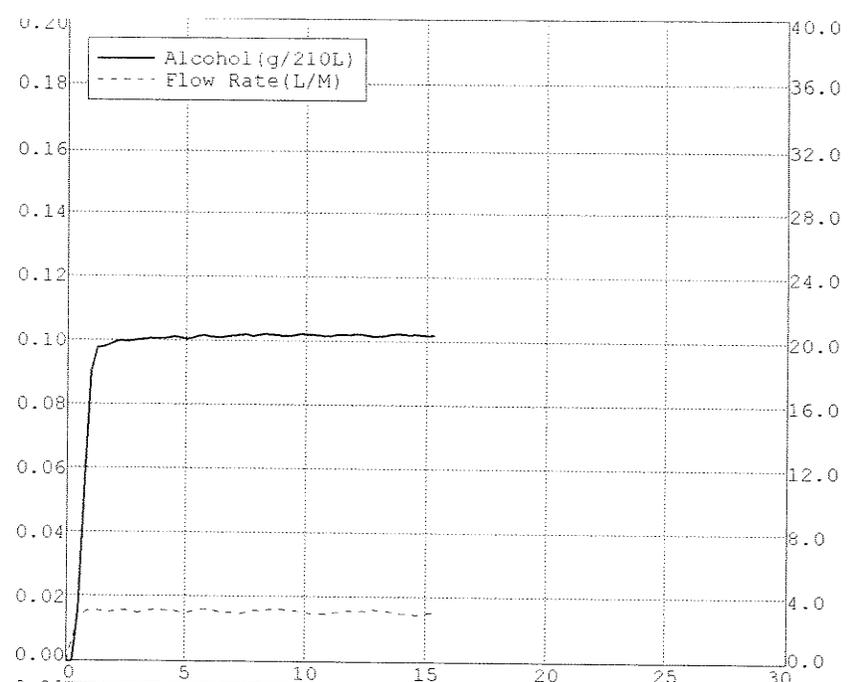

*Handwritten signature*