

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 07/29/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:03
INTERNAL STANDARD	VERIFIED	00:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:03
BLANK TEST	0.00	00:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:05
BLANK TEST	0.00	00:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:06
BLANK TEST	0.00	00:07

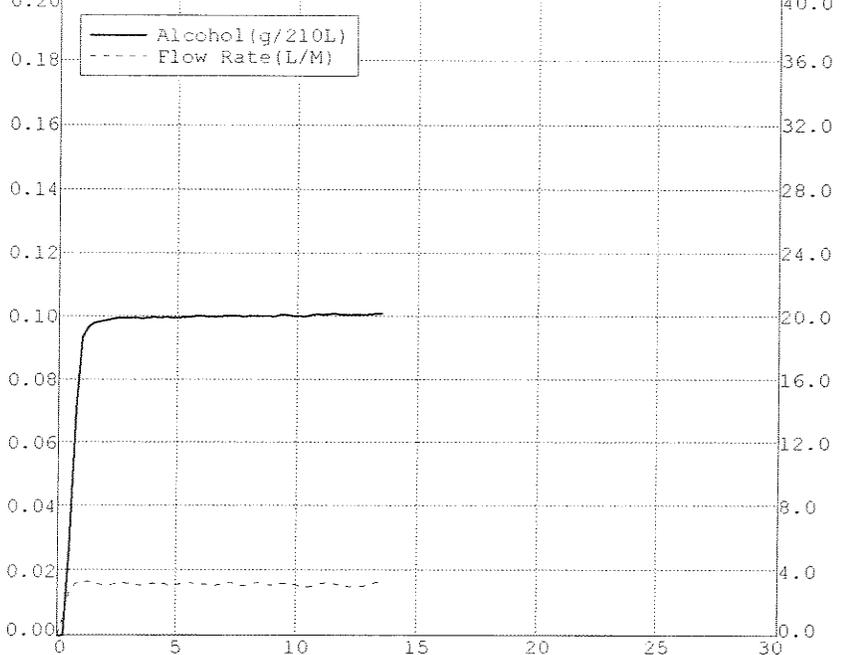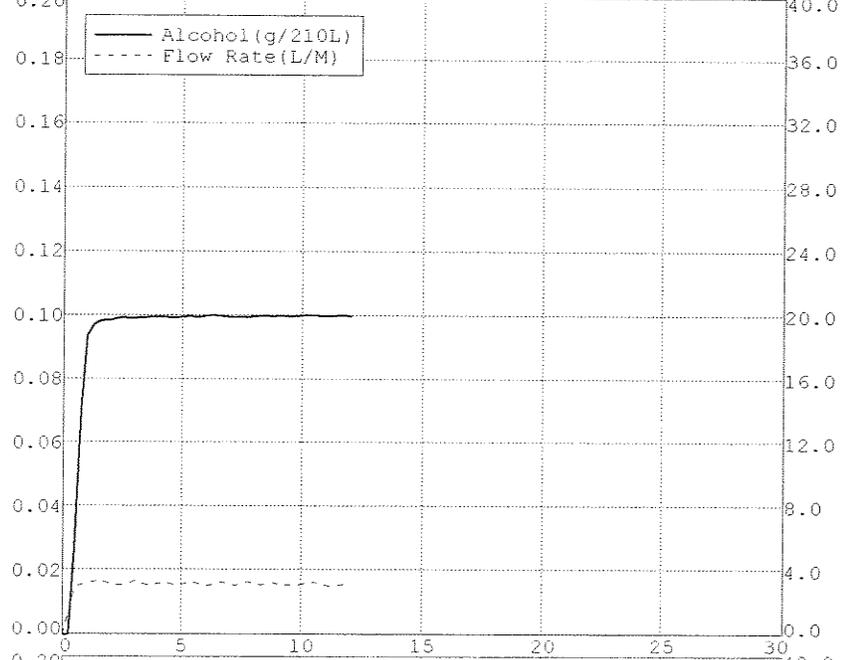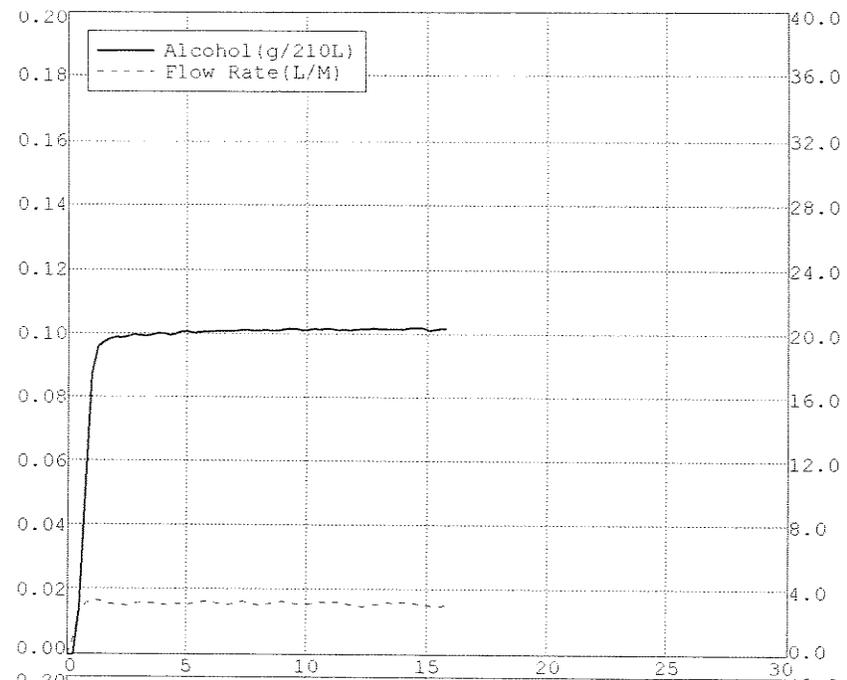

Charles B Geisler