

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 08/30/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18170

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:06
INTERNAL STANDARD	VERIFIED	06:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:06
BLANK TEST	0.00	06:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:07
BLANK TEST	0.00	06:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:09
BLANK TEST	0.00	06:10

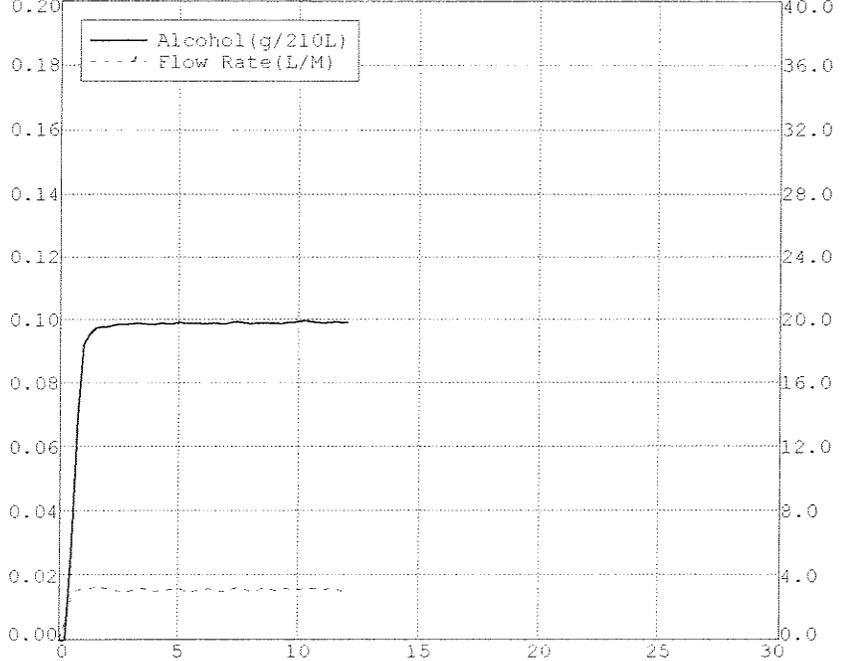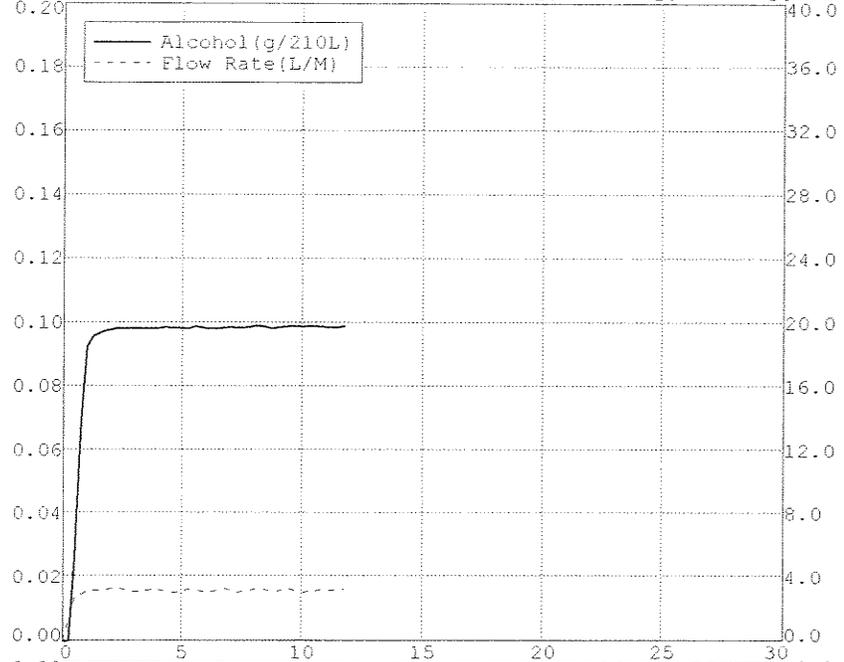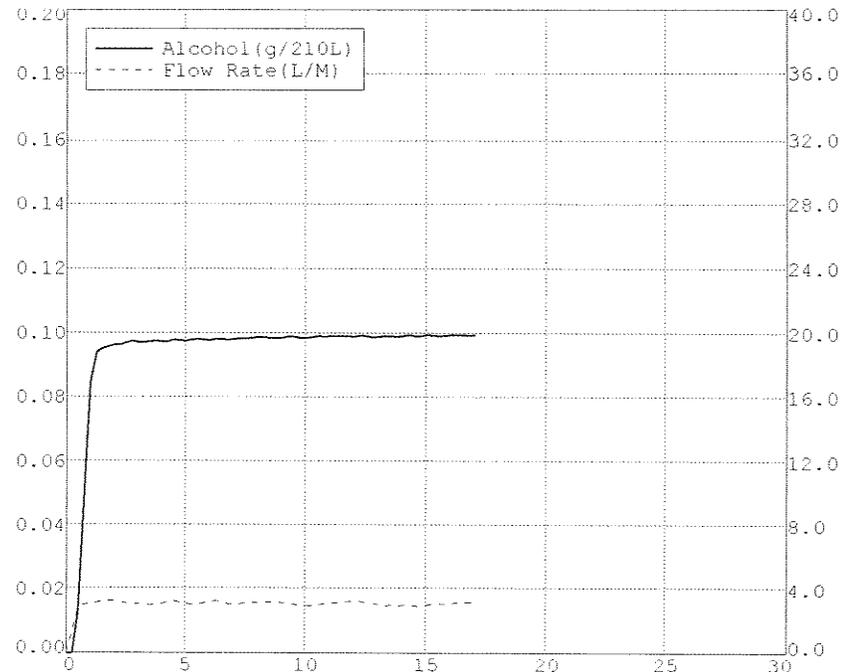

Ch. B. Geisler #24