

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 09/10/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18170

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:02
INTERNAL STANDARD	VERIFIED	01:02
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	01:02
BLANK TEST	0.00	01:03
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	01:03
BLANK TEST	0.00	01:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	01:05
BLANK TEST	0.00	01:05

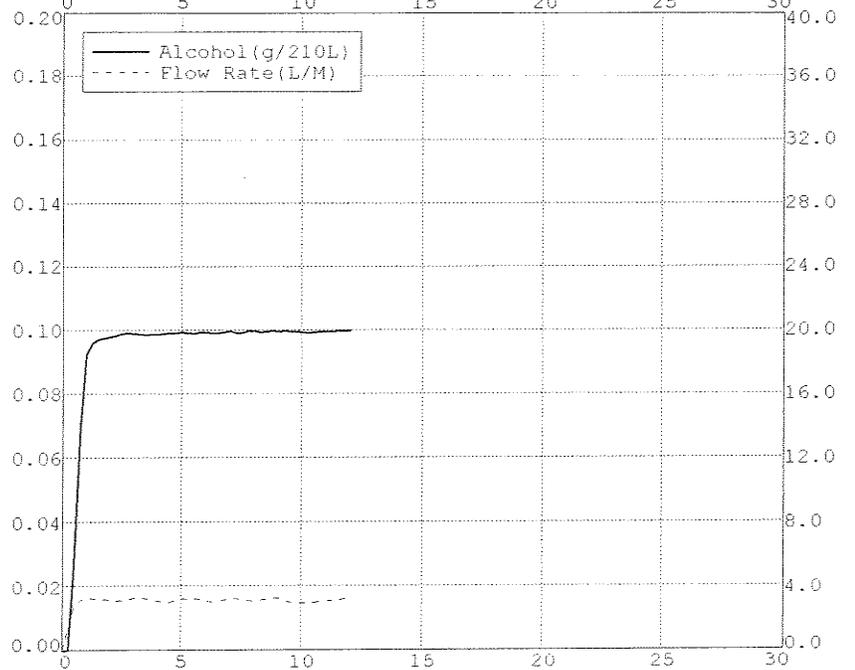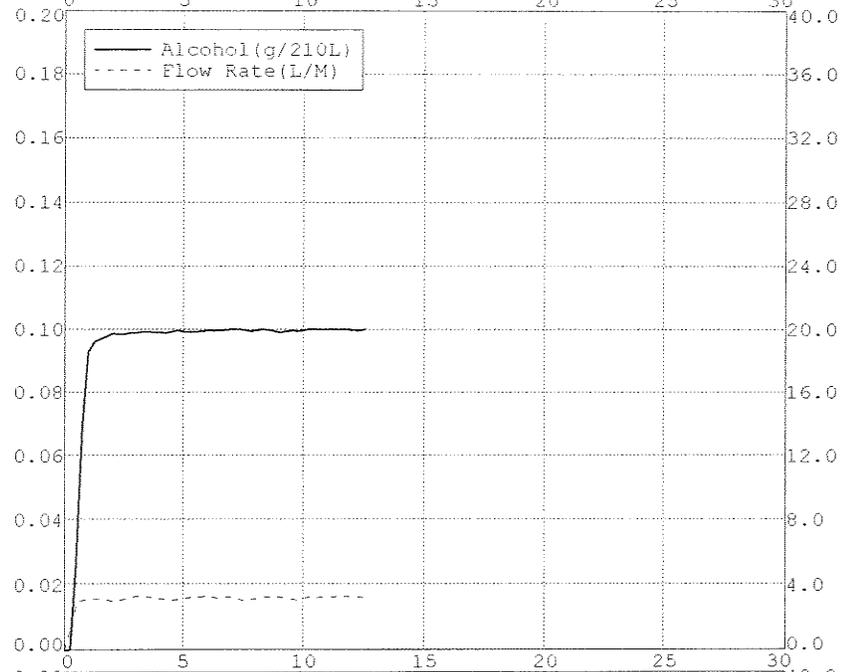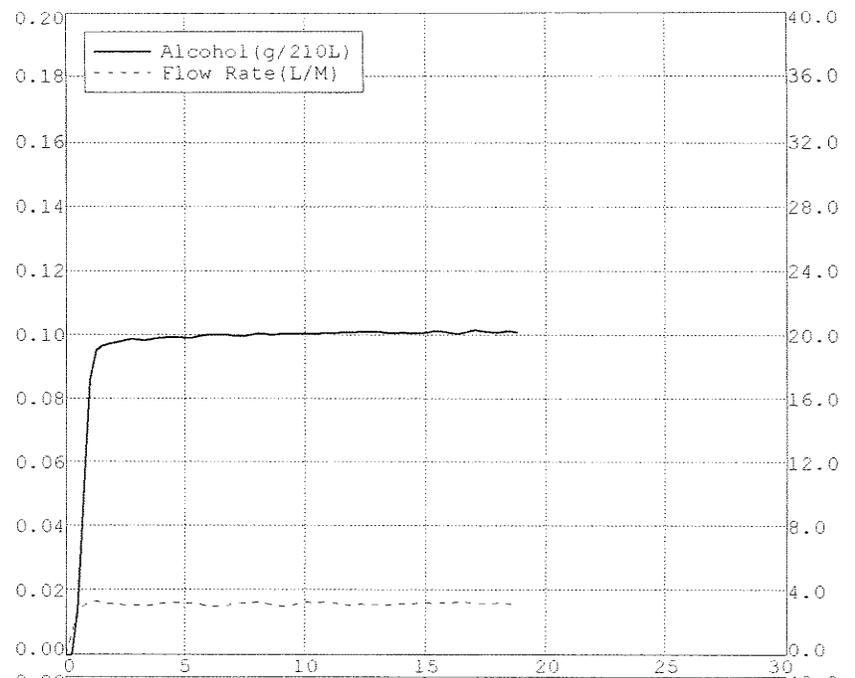

*Signature*