

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/19/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18170

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:18
INTERNAL STANDARD	VERIFIED	06:18
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	06:19
BLANK TEST	0.00	06:19
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	06:20
BLANK TEST	0.00	06:21
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	06:21
BLANK TEST	0.00	06:22

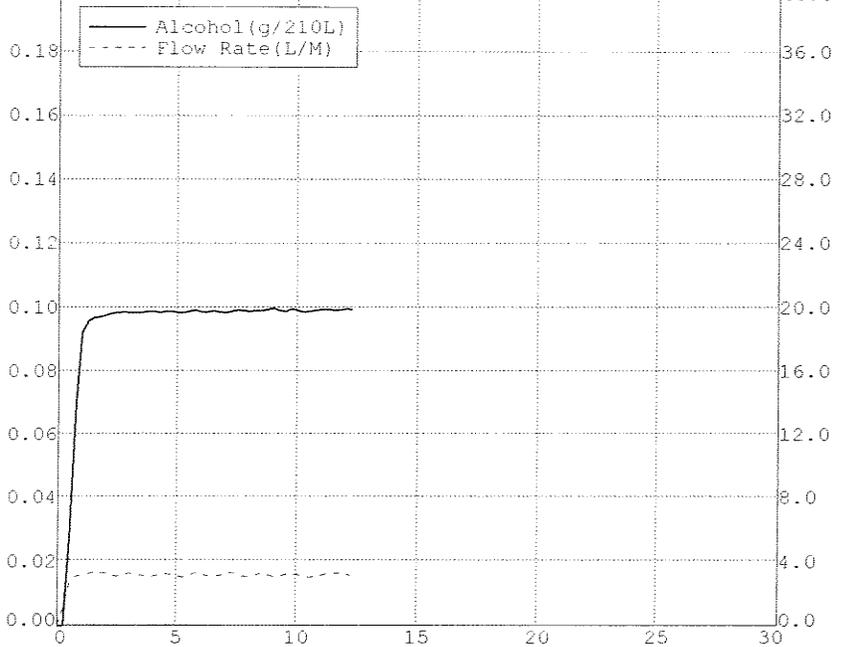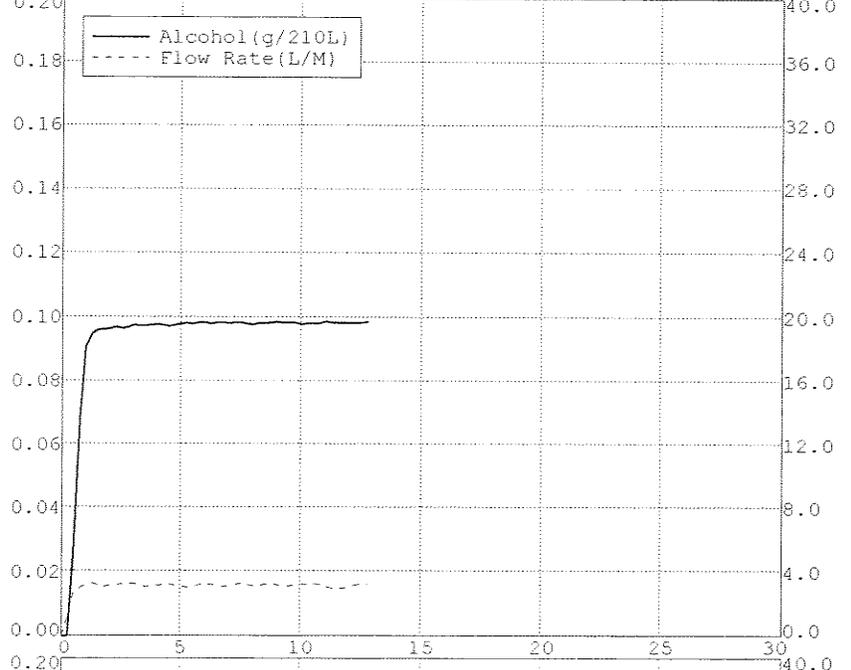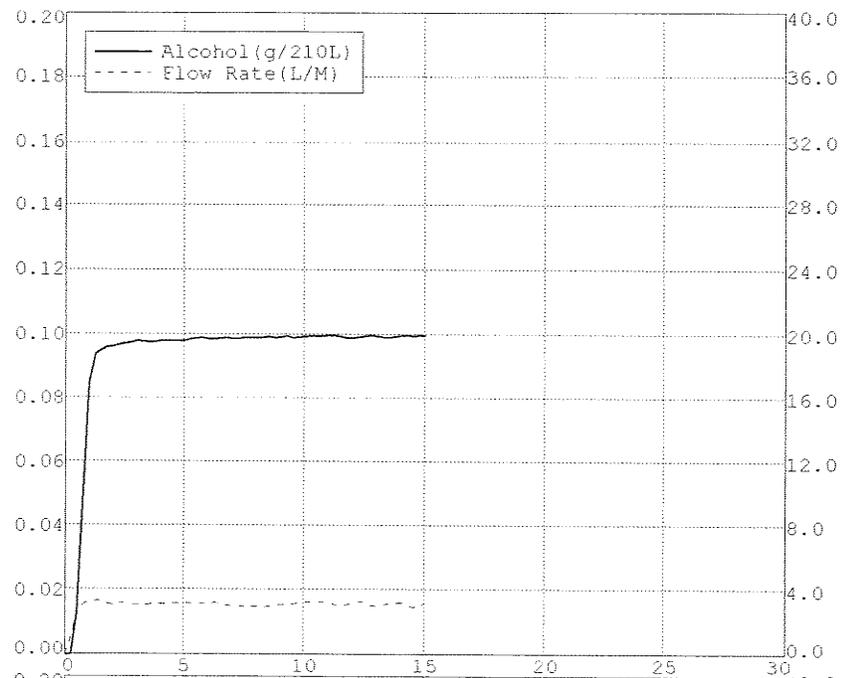

Charles B Geisler #241