

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 10/02/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:48
INTERNAL STANDARD	VERIFIED	02:48
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	02:48
BLANK TEST	0.00	02:49
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	02:50
BLANK TEST	0.00	02:51
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	02:51
BLANK TEST	0.00	02:52

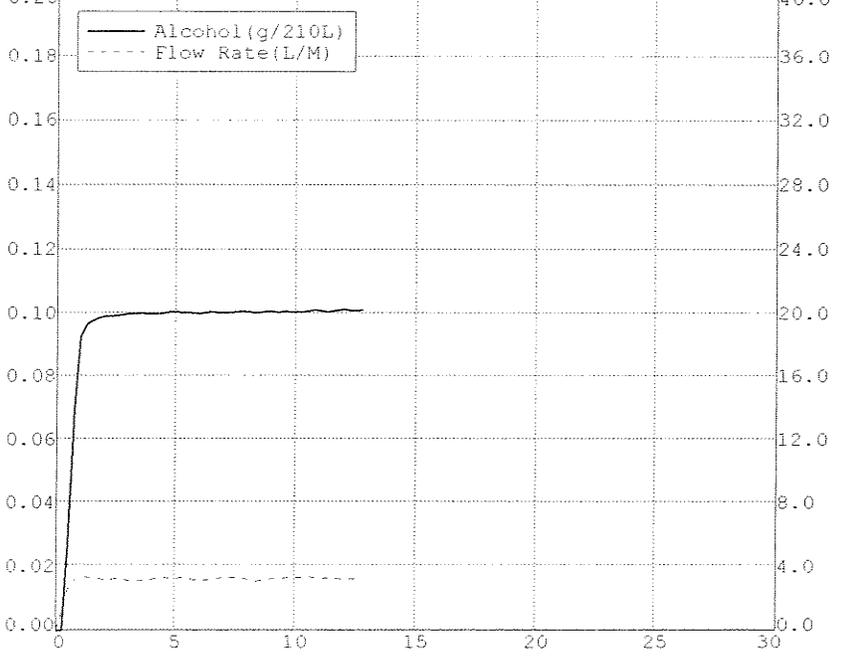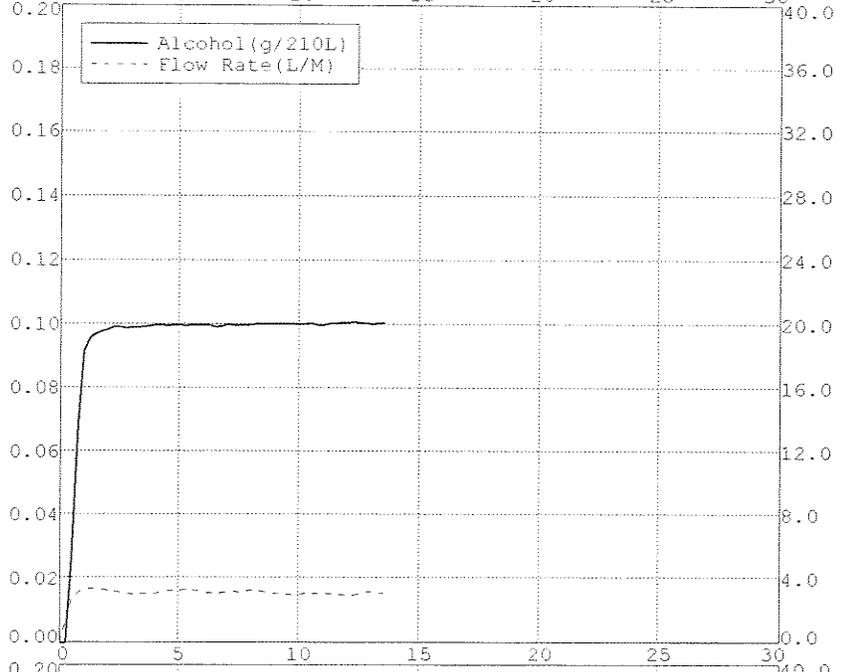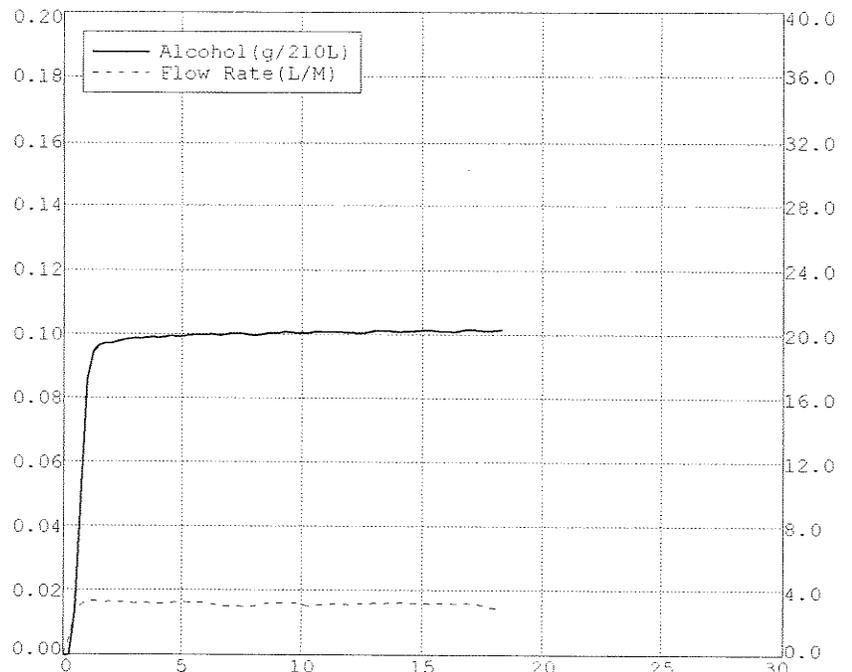

Charles B. Geisler *AG* *AG*