

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 10/08/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:34
INTERNAL STANDARD	VERIFIED	03:34
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	03:34
BLANK TEST	0.00	03:35
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	03:36
BLANK TEST	0.00	03:36
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	03:37
BLANK TEST	0.00	03:38

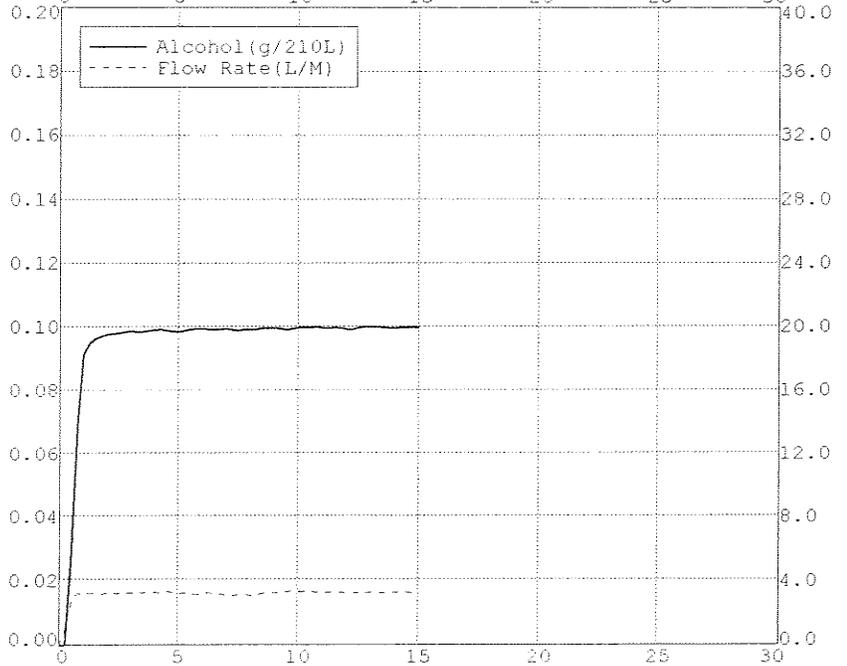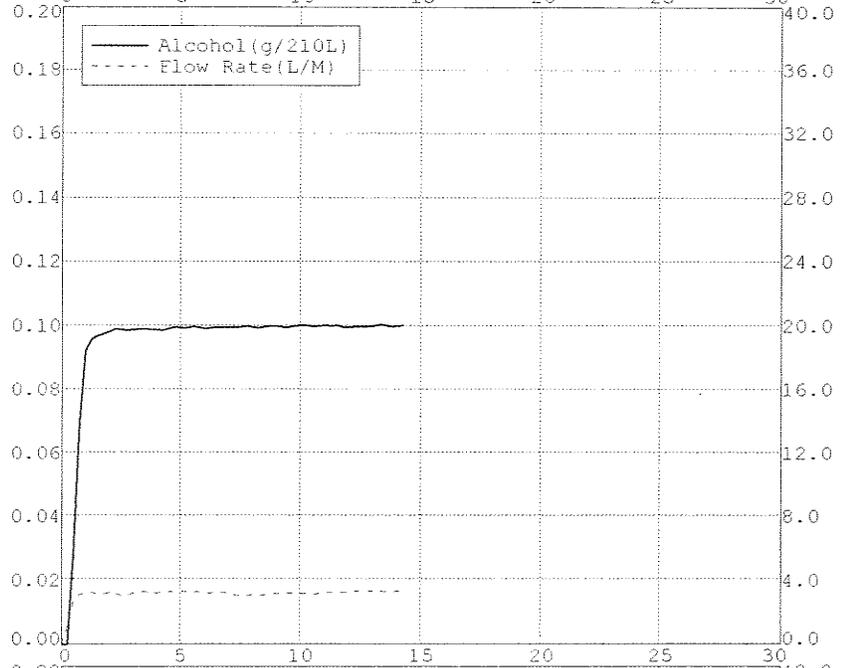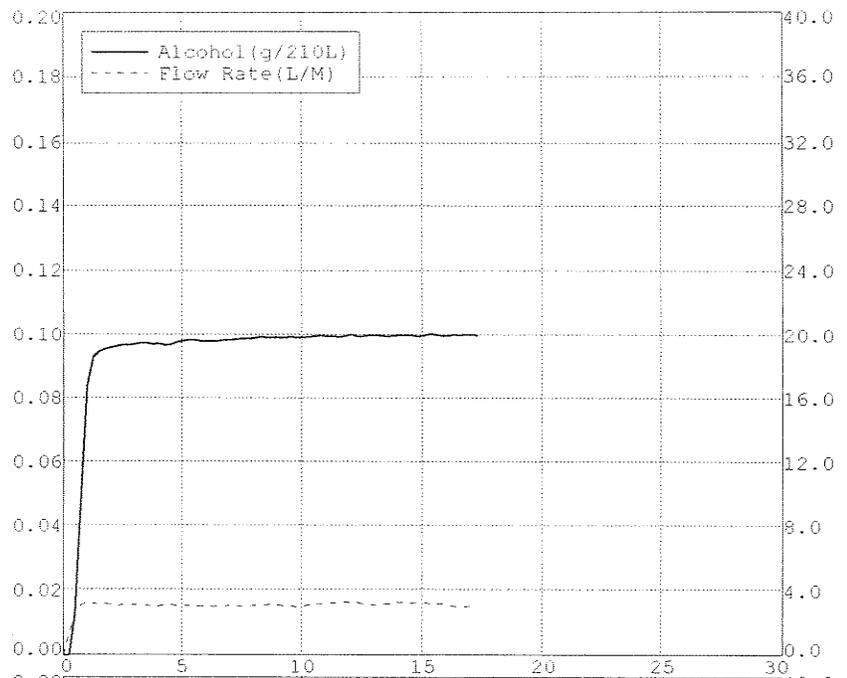

*Charles B. Geisler*