

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 10/15/2018

OPERATOR NAME:  
J T COON  
Permit #: 36043  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:04
INTERNAL STANDARD	VERIFIED	06:05
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	06:05
BLANK TEST	0.00	06:06
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	06:06
BLANK TEST	0.00	06:07
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	06:08
BLANK TEST	0.00	06:08

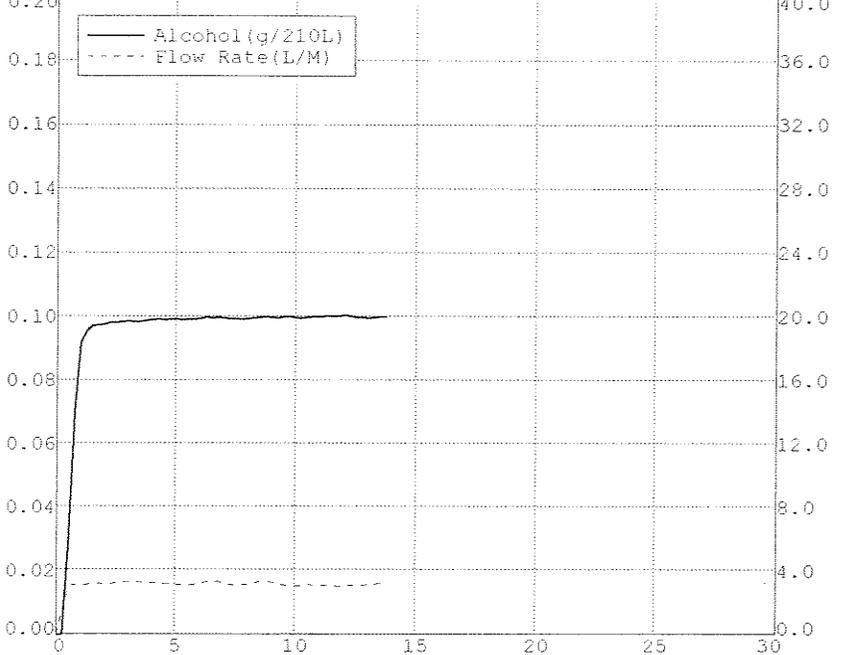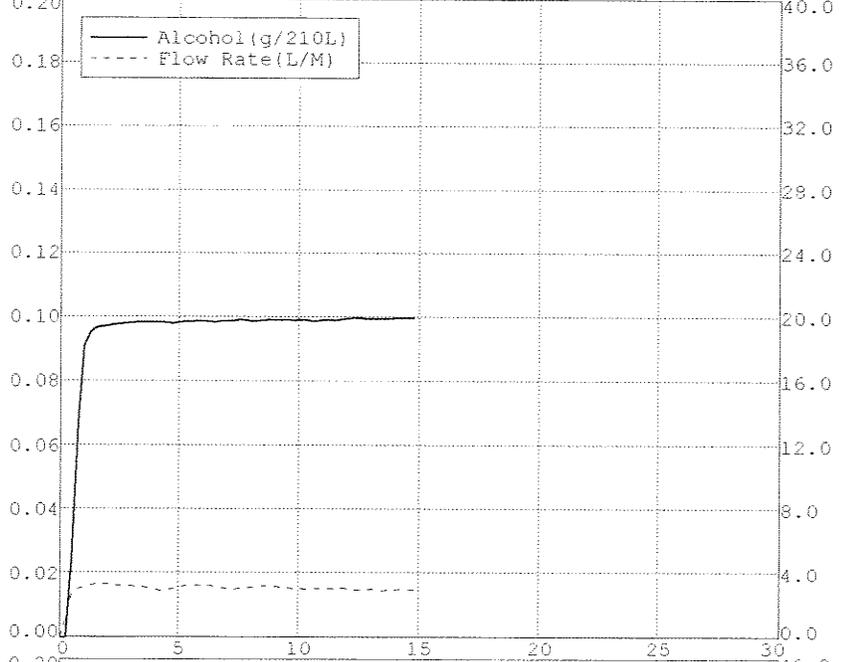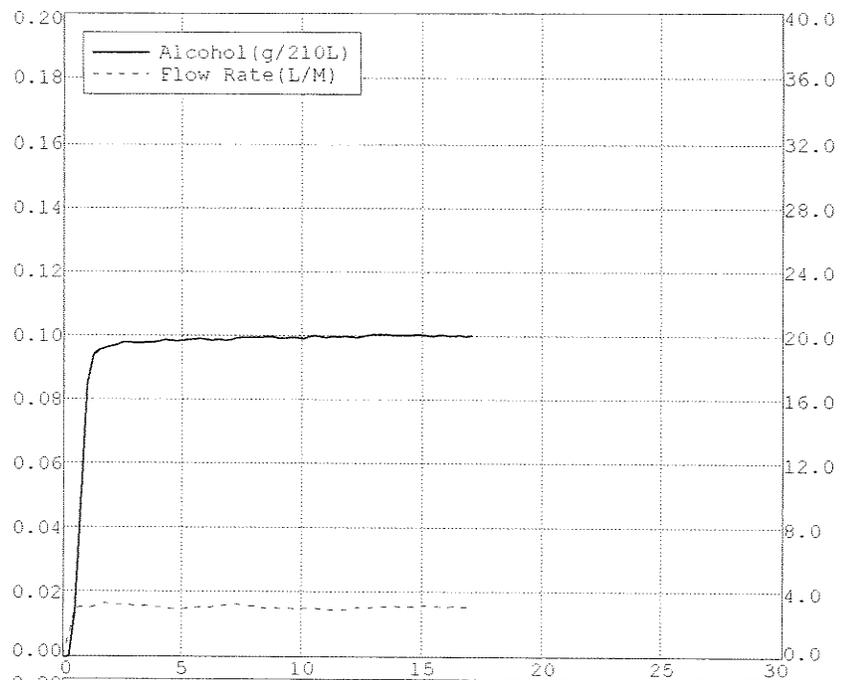

*Handwritten signature: J T Coon*