

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 10/22/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:08
INTERNAL STANDARD	VERIFIED	04:08
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	04:08
BLANK TEST	0.00	04:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	04:10
BLANK TEST	0.00	04:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	04:11
BLANK TEST	0.00	04:12

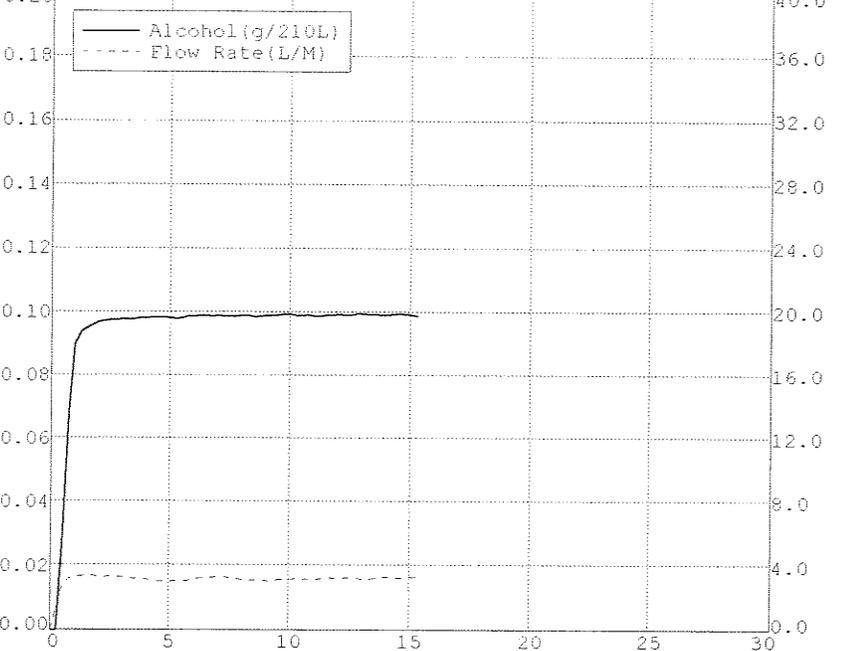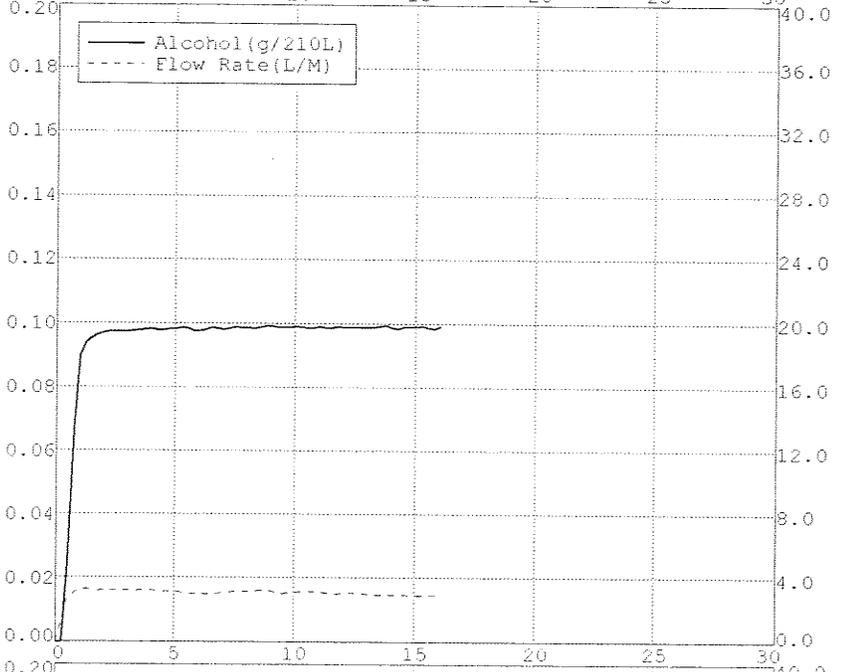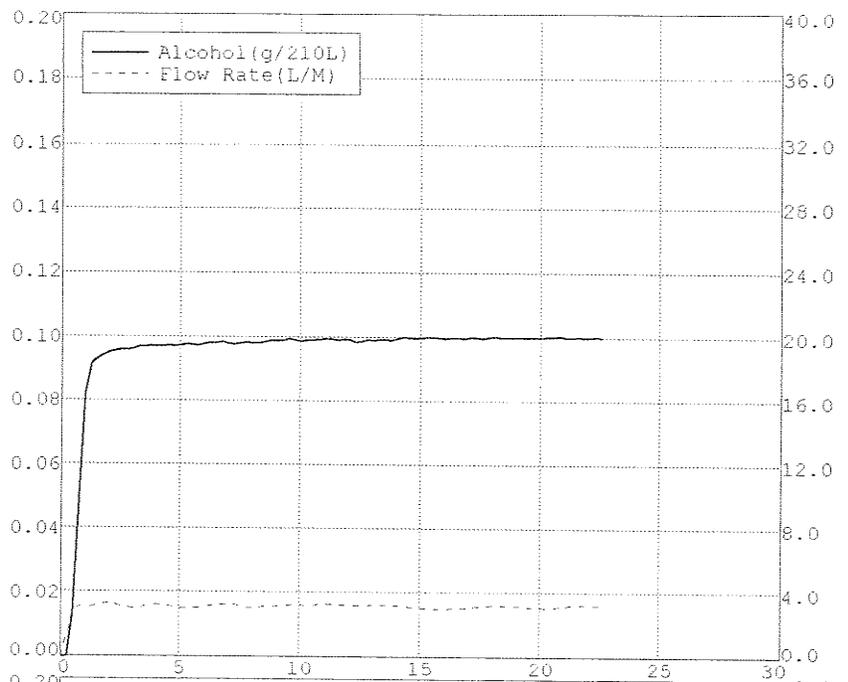

Sgt. Charles B. Geisler