

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 10/30/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:54
INTERNAL STANDARD	VERIFIED	13:55
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	13:55
BLANK TEST	0.00	13:56
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	13:56
BLANK TEST	0.00	13:57
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	13:58
BLANK TEST	0.00	13:58

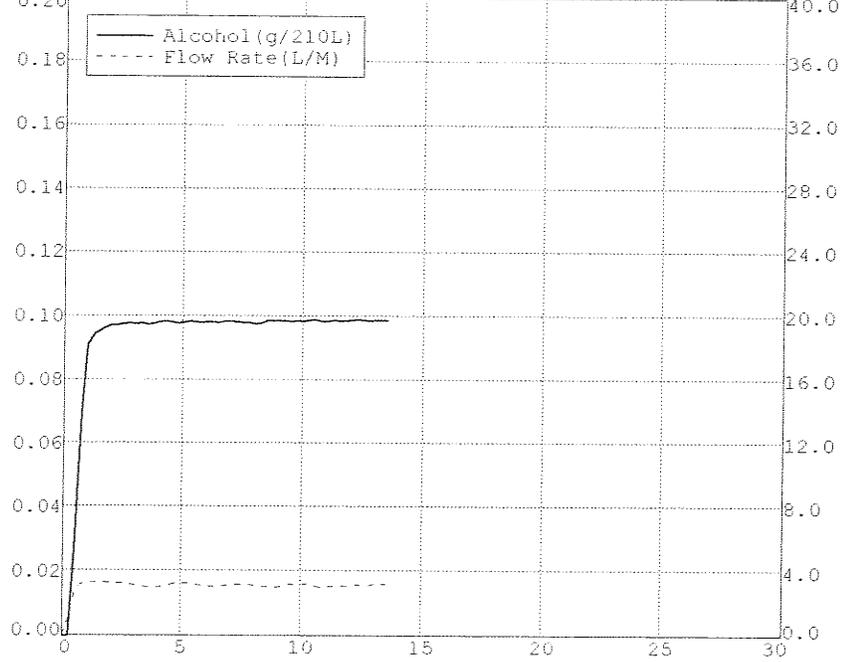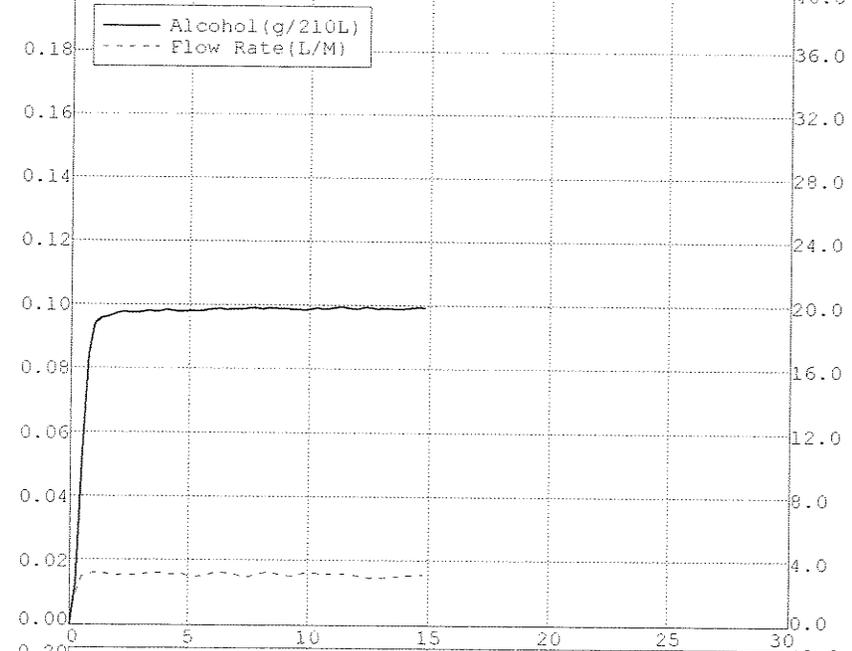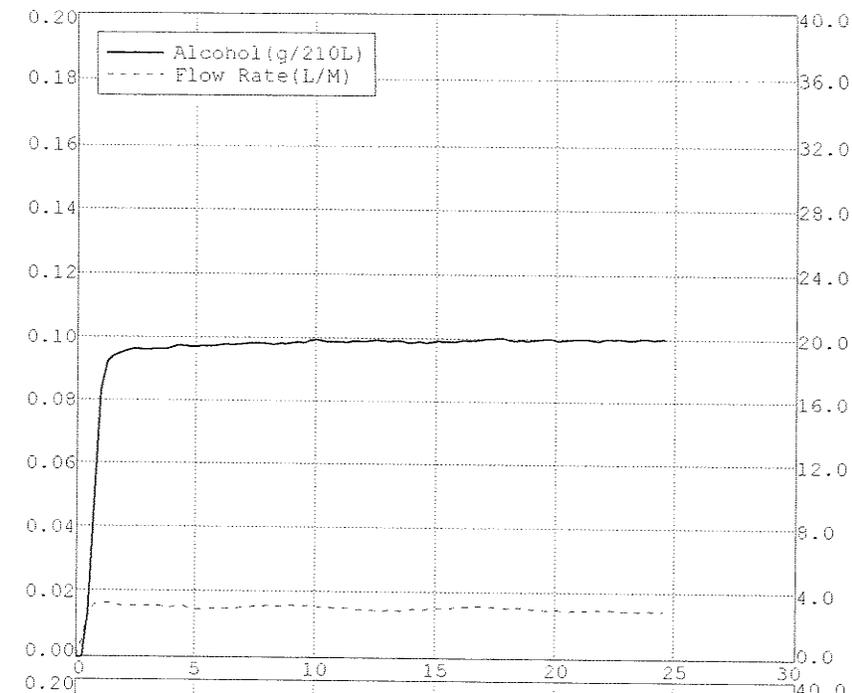

*Geisler* *LL* #241