

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 11/01/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:43
INTERNAL STANDARD	VERIFIED	12:43
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.10	12:44
BLANK TEST	0.00	12:45
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.10	12:45
BLANK TEST	0.00	12:46
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:46
BLANK TEST	0.00	12:47

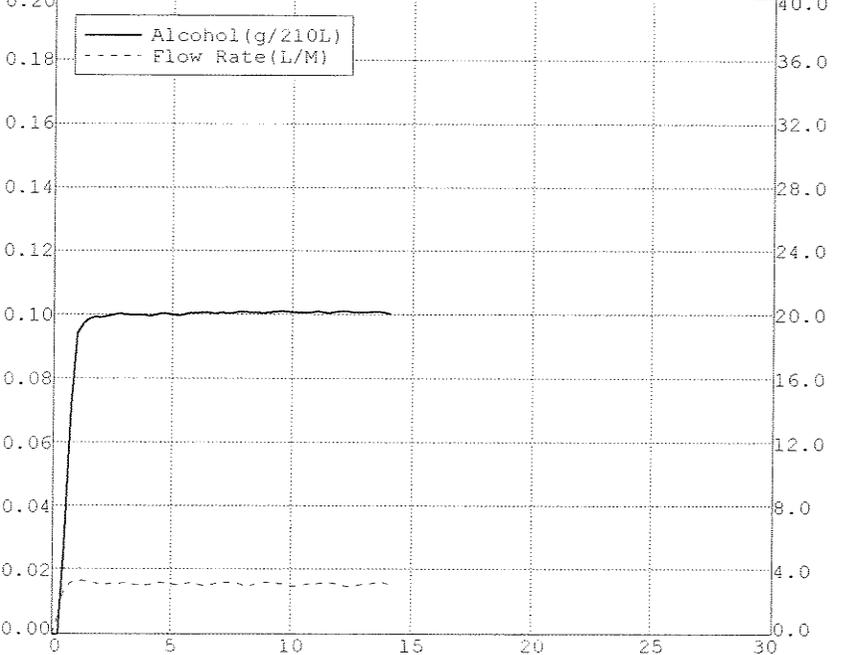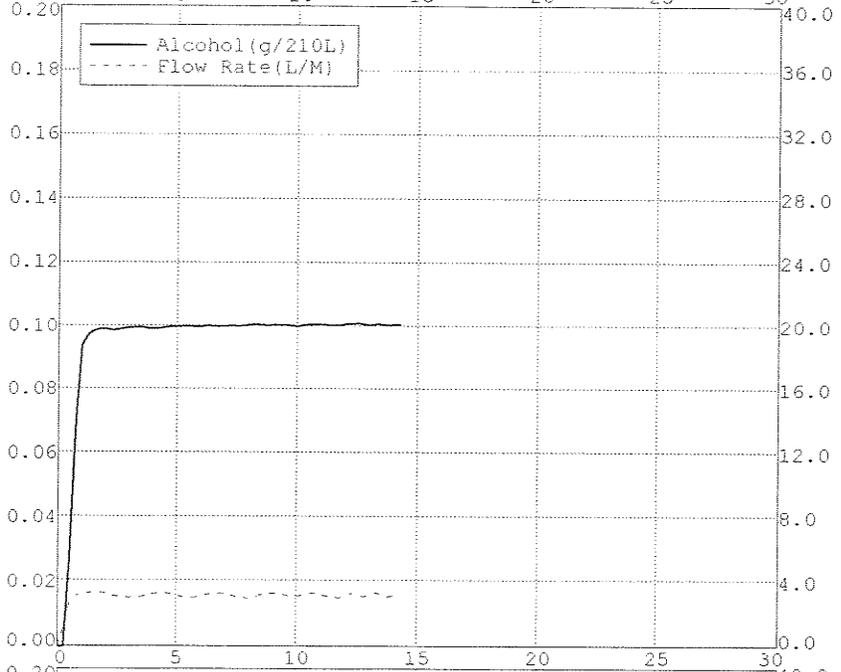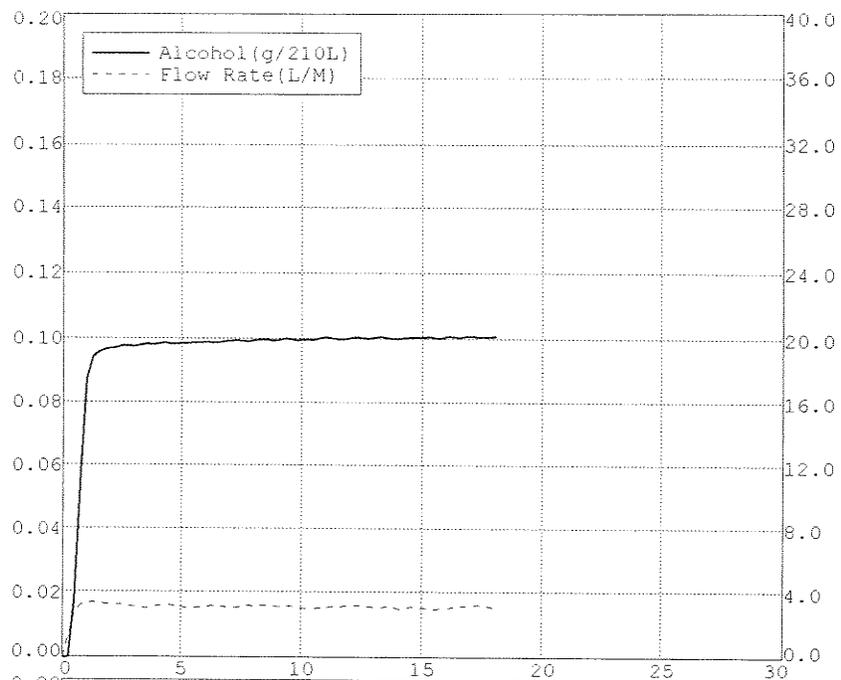

Handwritten signature: C. B. Geisler