

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 11/14/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:00
INTERNAL STANDARD	VERIFIED	04:01
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	04:01
BLANK TEST	0.00	04:02
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	04:02
BLANK TEST	0.00	04:03
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	04:03
BLANK TEST	0.00	04:04

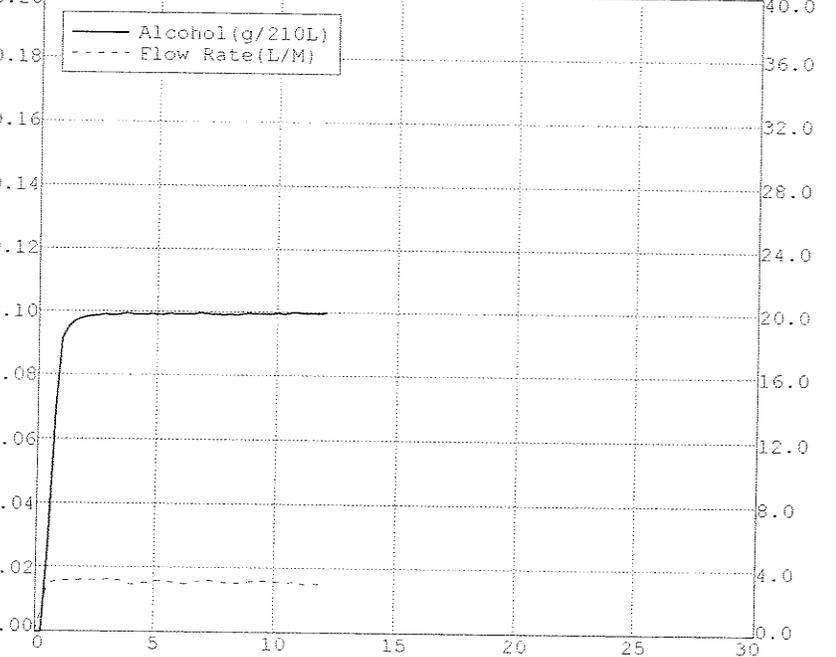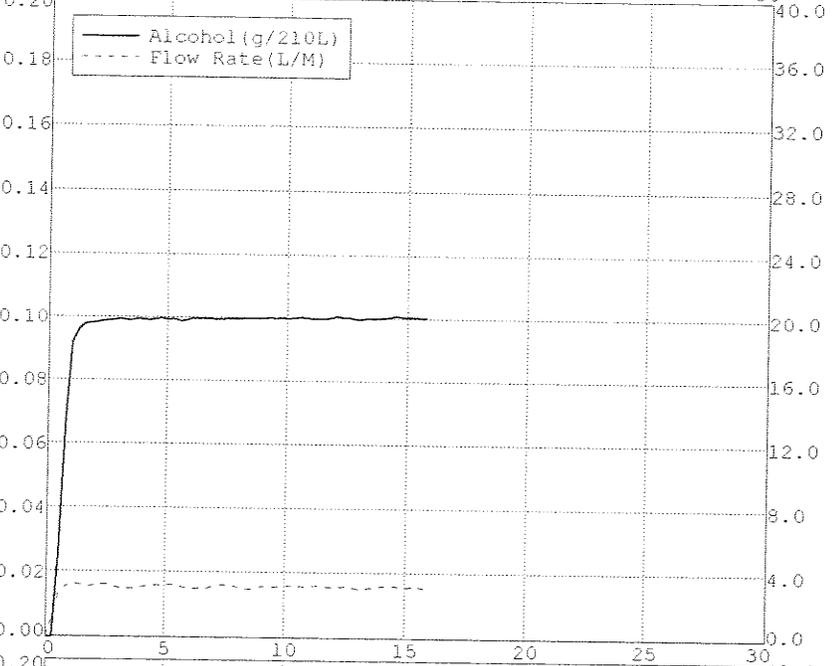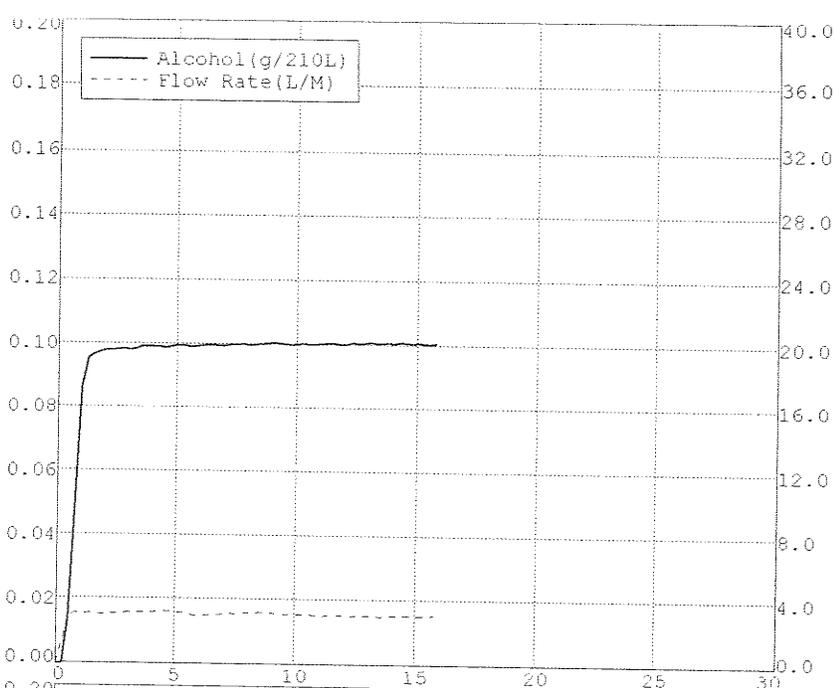

Charles B Geisler #24