

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 12/05/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:08
INTERNAL STANDARD	VERIFIED	21:08
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	21:09
BLANK TEST	0.00	21:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:10
BLANK TEST	0.00	21:11
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:11
BLANK TEST	0.00	21:12

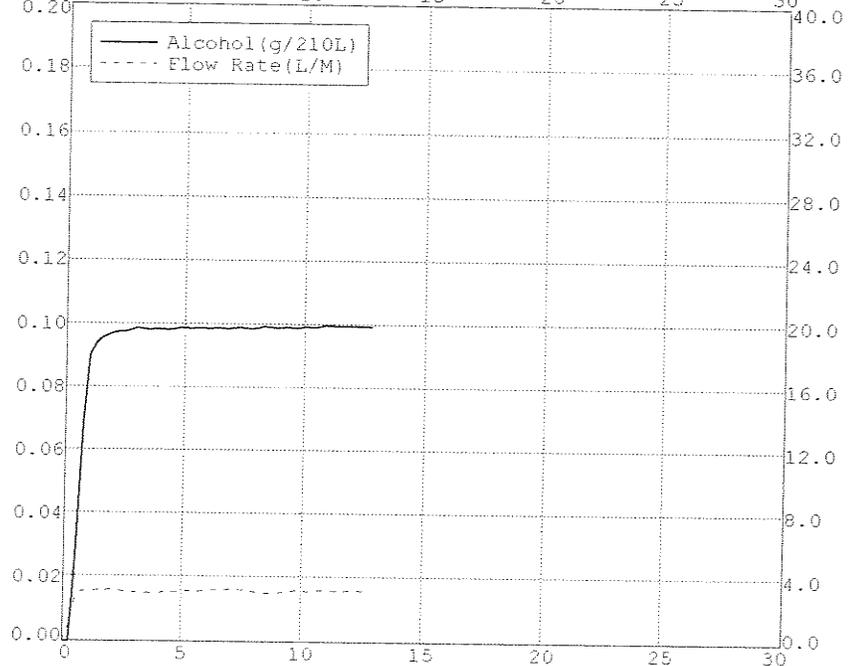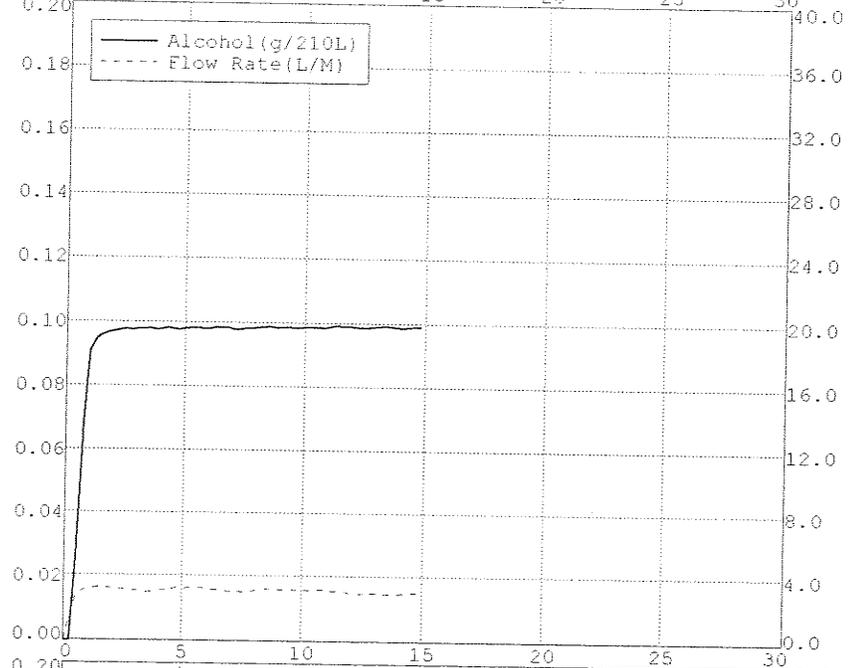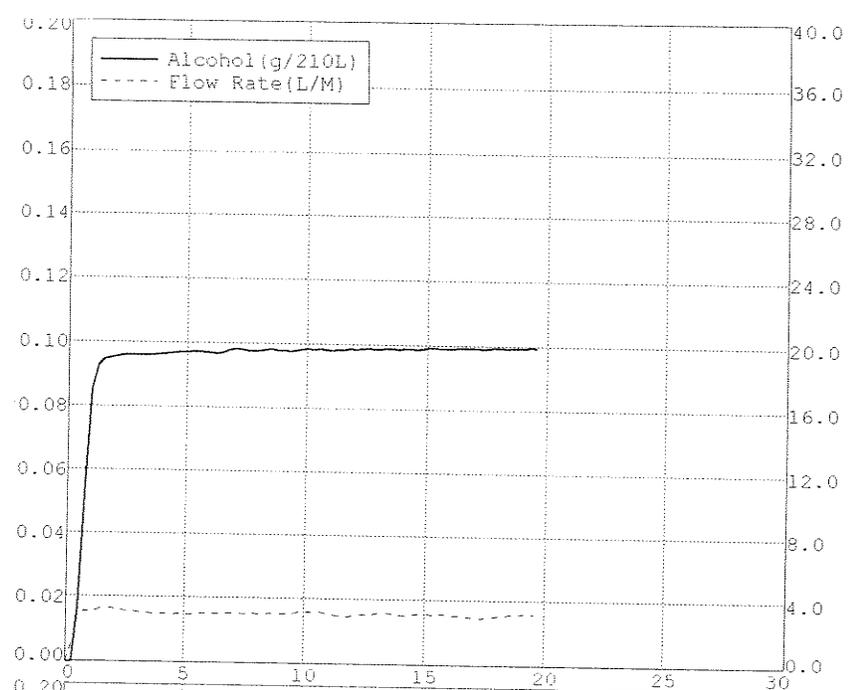

Charles B Geisler #241