

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 12/20/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:15
INTERNAL STANDARD	VERIFIED	01:15
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	01:15
BLANK TEST	0.00	01:16
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:16
BLANK TEST	0.00	01:17
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	01:17
BLANK TEST	0.00	01:18

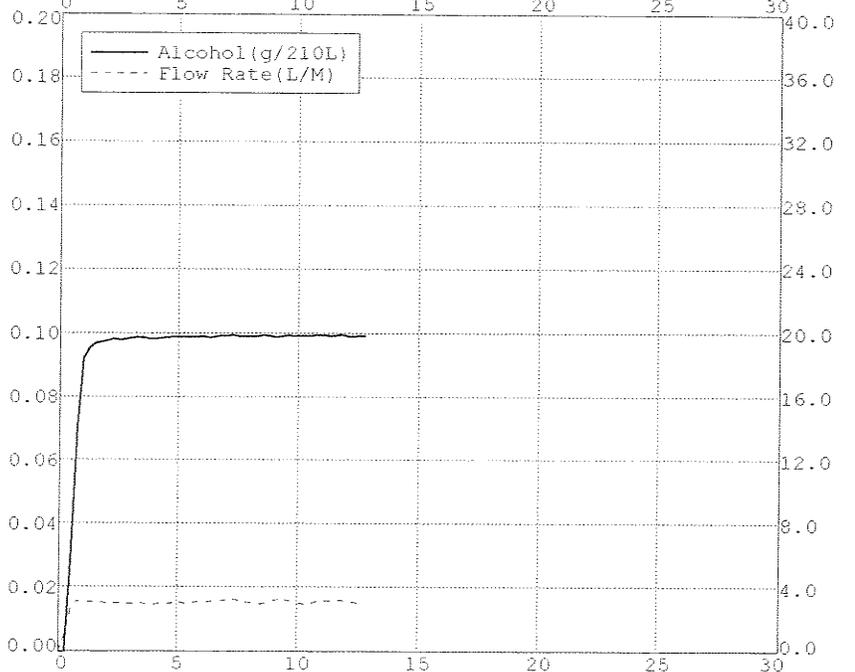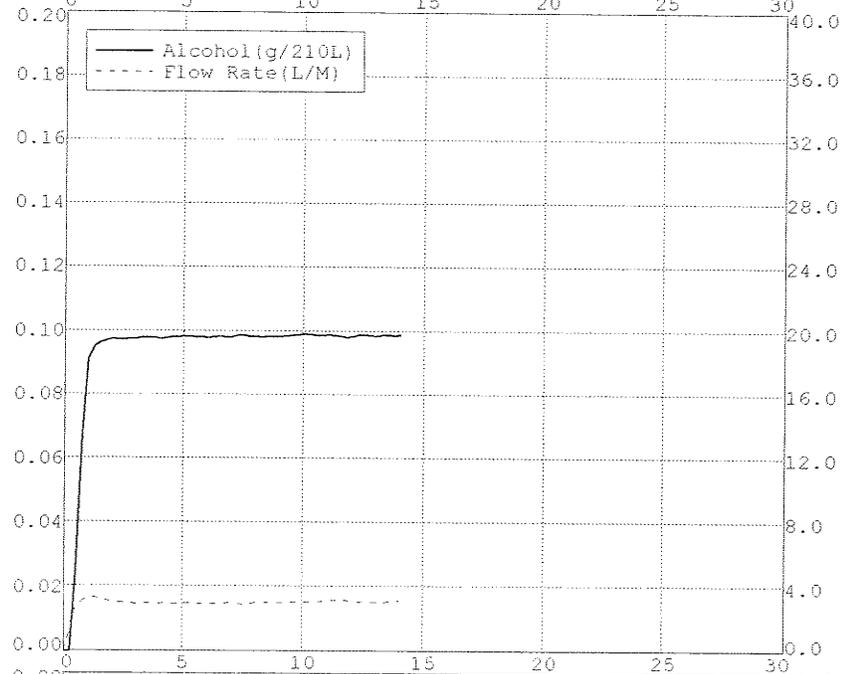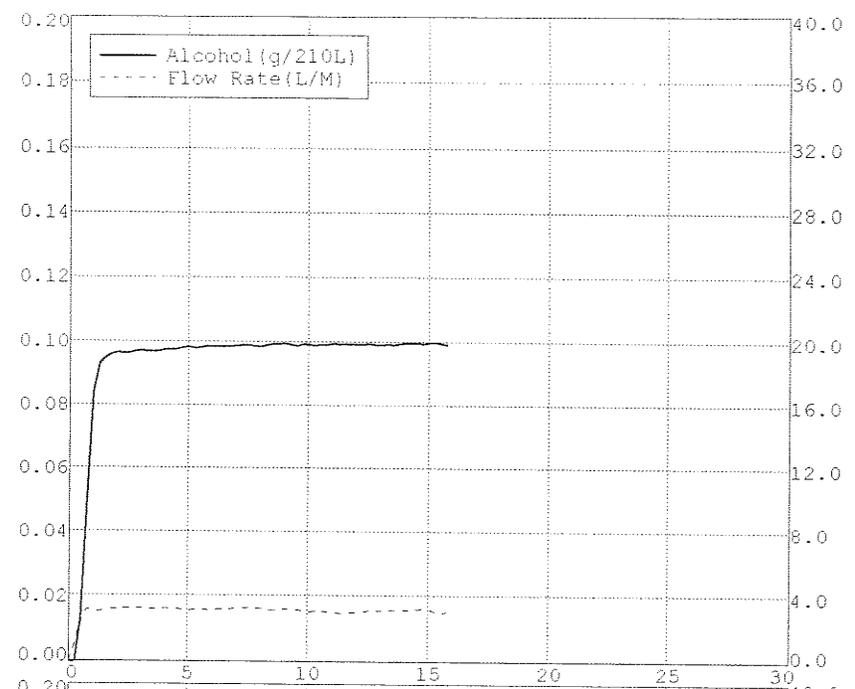

Charles B. Geisler #241