

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 12/26/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:57
INTERNAL STANDARD	VERIFIED	02:57
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:58
BLANK TEST	0.00	02:59
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:59
BLANK TEST	0.00	03:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:00
BLANK TEST	0.00	03:01

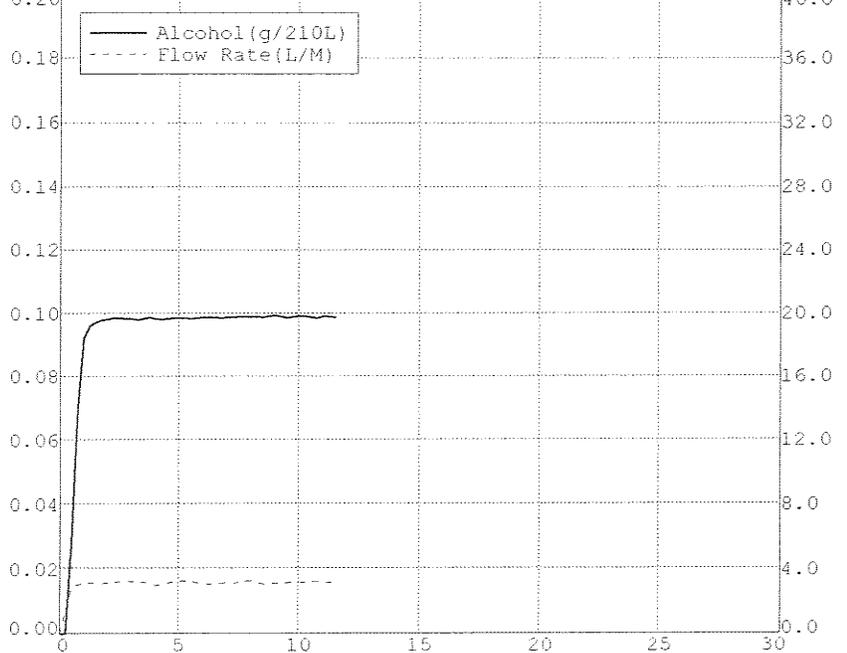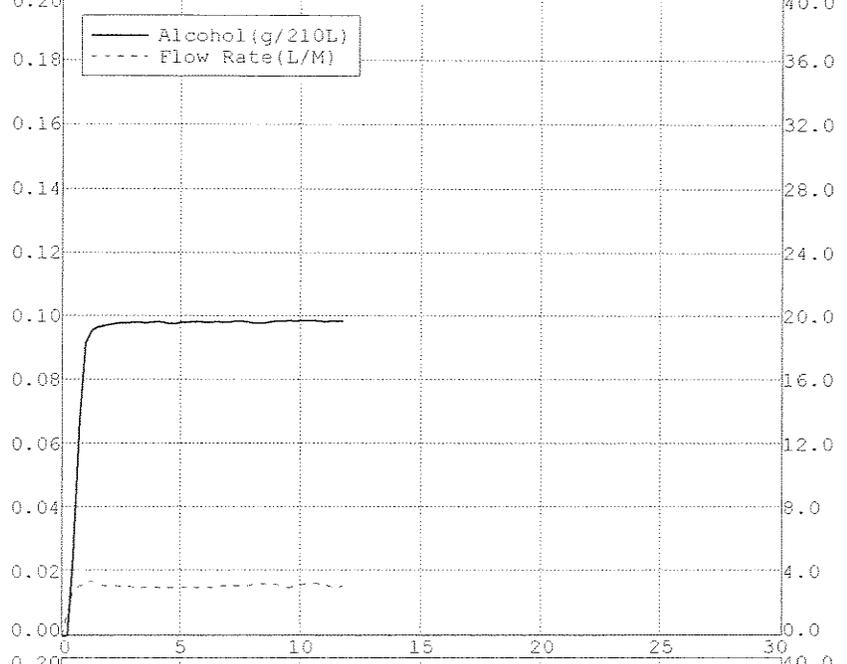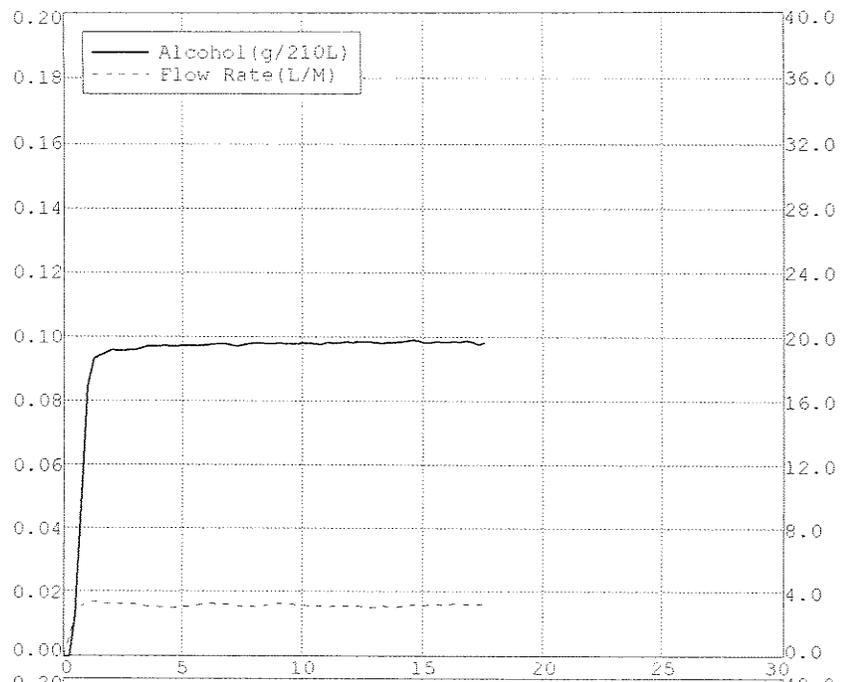

*Charles B Geisler* #24