

SUPERVISOR TEST




 WARREN COUNTY
 SHERRIF'S OFFICE
 DATAMASTER dmt: 144506

Date: 01/13/2018

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:12
INTERNAL STANDARD	VERIFIED	23:12
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	23:12
BLANK TEST	0.00	23:13
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	23:13
BLANK TEST	0.00	23:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:14
BLANK TEST	0.00	23:15

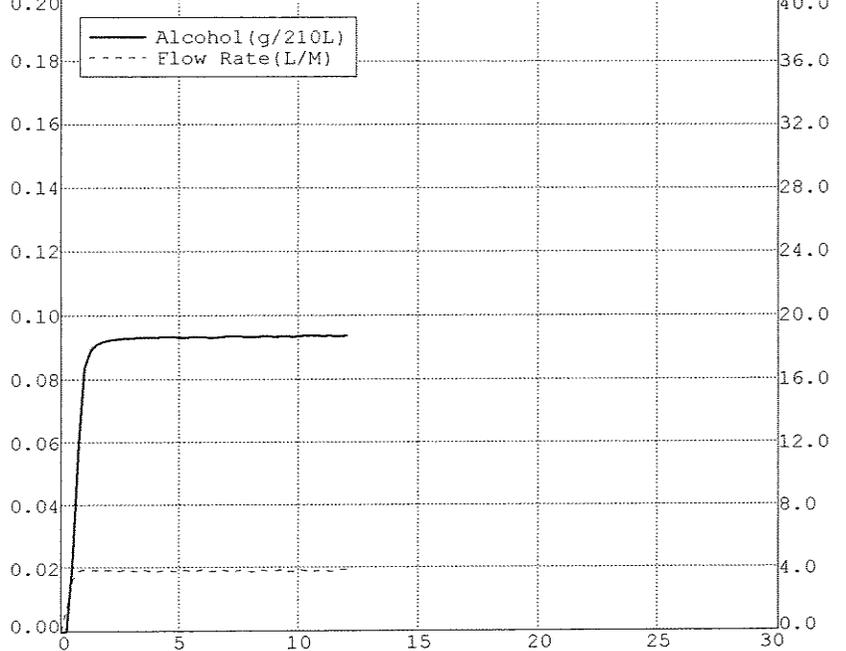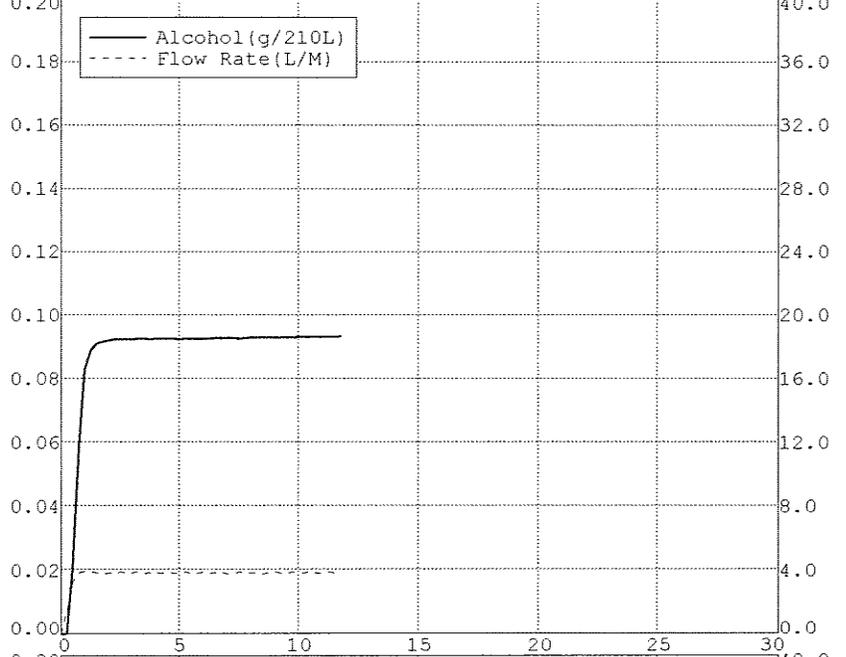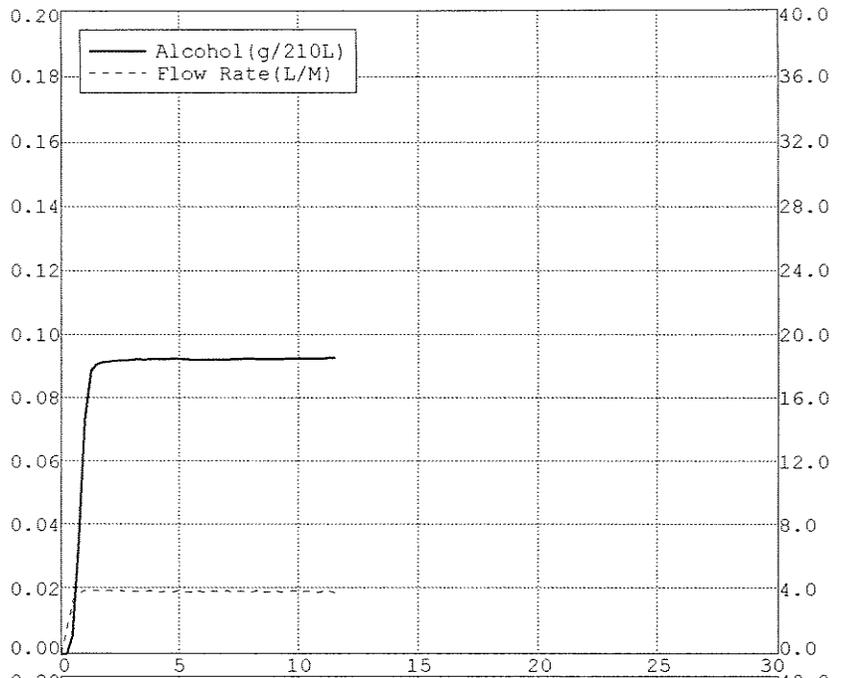

Charles B. Geisler #244