

SUPERVISOR TEST




WARREN COUNTY  
SHERRIF'S OFFICE  
DATAMASTER dmt: 144506

Date: 01/19/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:49
INTERNAL STANDARD	VERIFIED	00:49
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:49
BLANK TEST	0.00	00:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:50
BLANK TEST	0.00	00:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:51
BLANK TEST	0.00	00:52

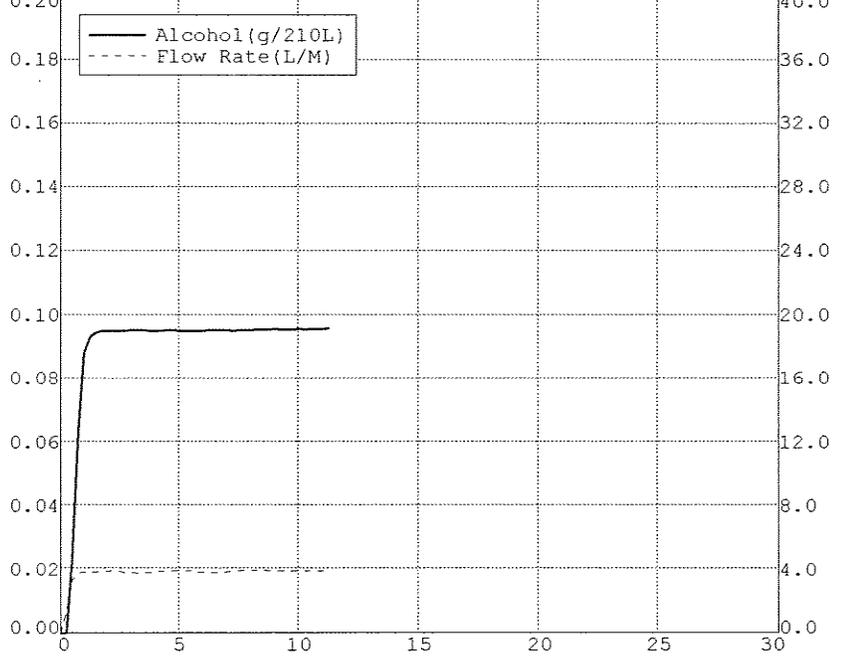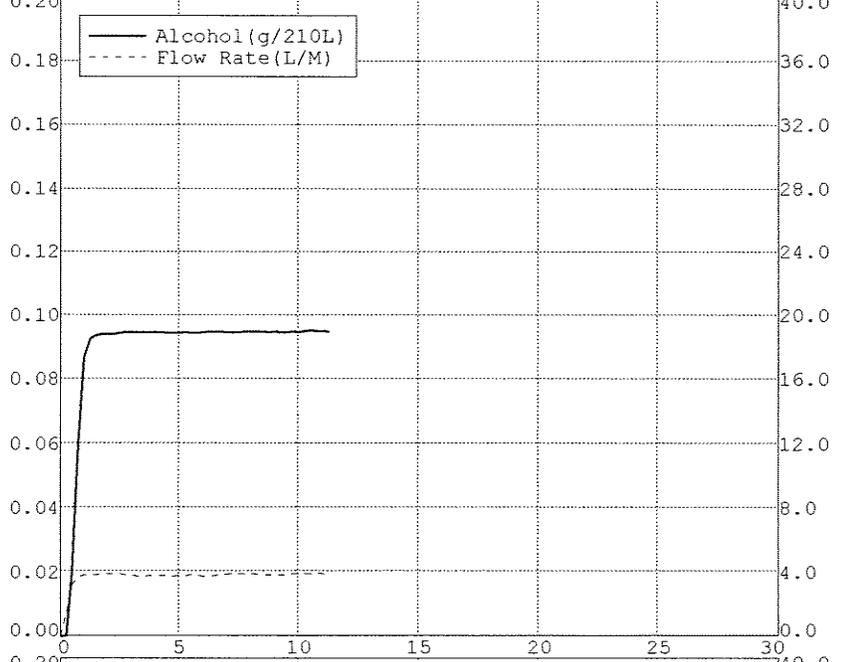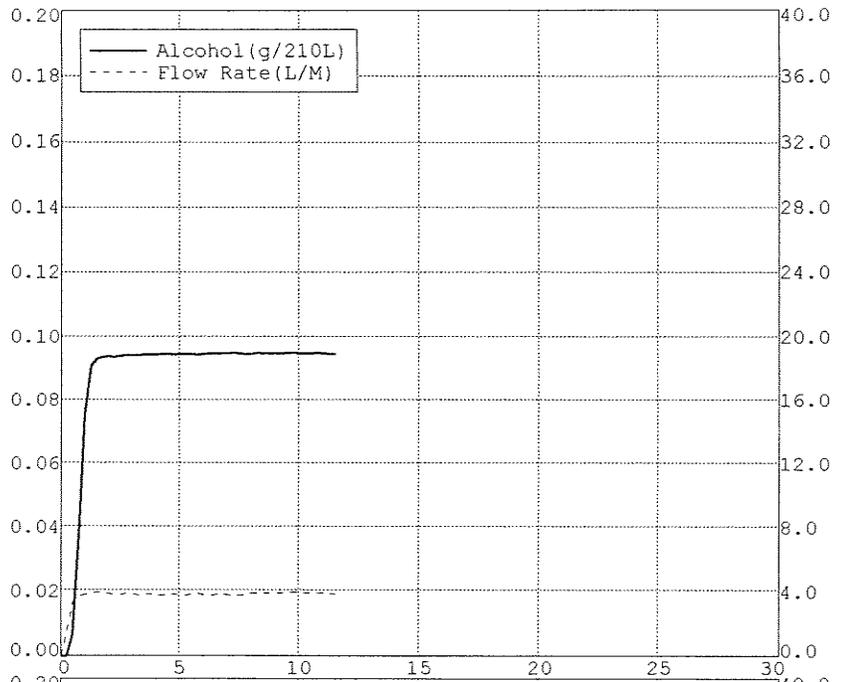

*Charles B. Geisler* #2246