

SUPERVISOR TEST




WARREN COUNTY
SHERRIF'S OFFICE
DATAMASTER dmt: 144506

Date: 02/16/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:39
INTERNAL STANDARD	VERIFIED	02:40
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:40
BLANK TEST	0.00	02:41
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	02:41
BLANK TEST	0.00	02:42
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	02:42
BLANK TEST	0.00	02:43

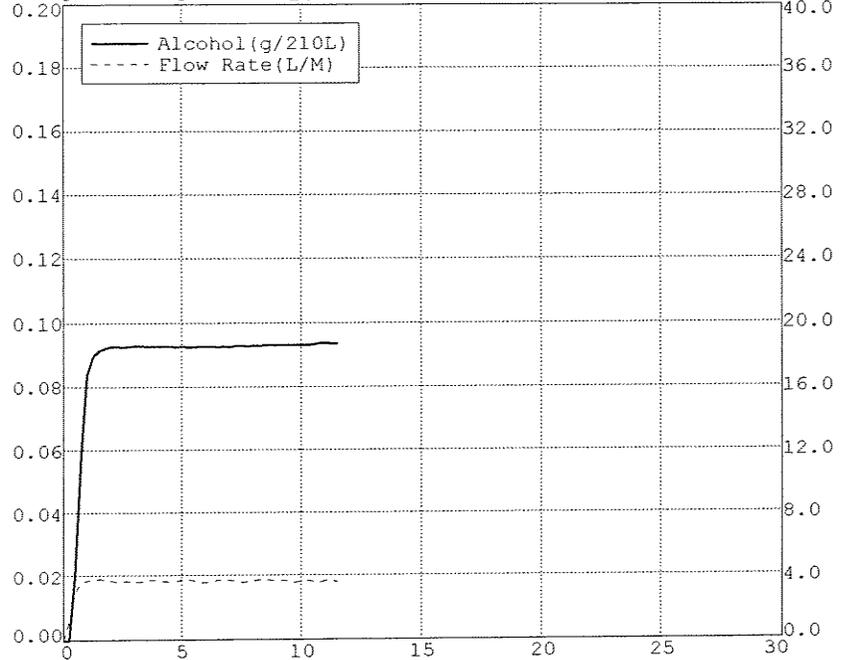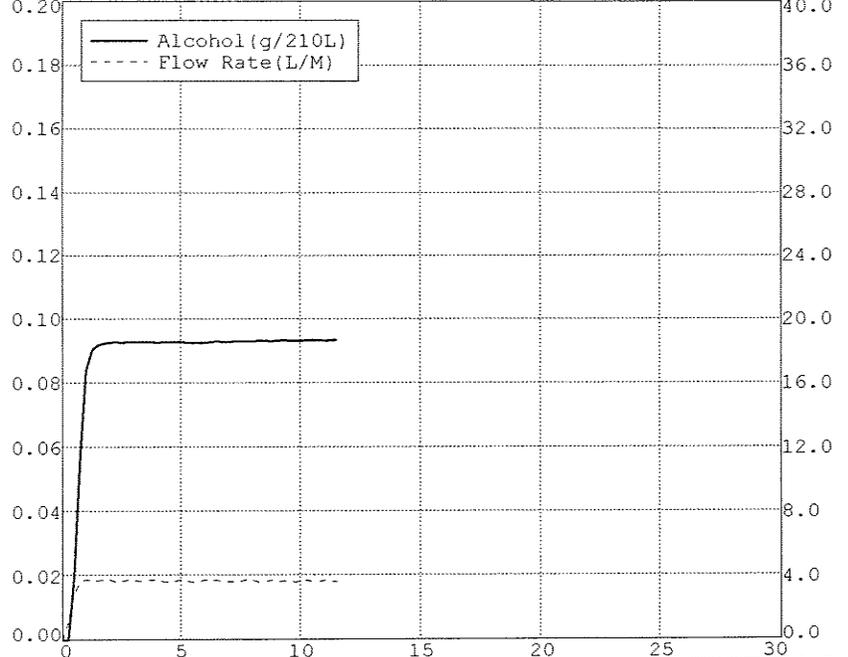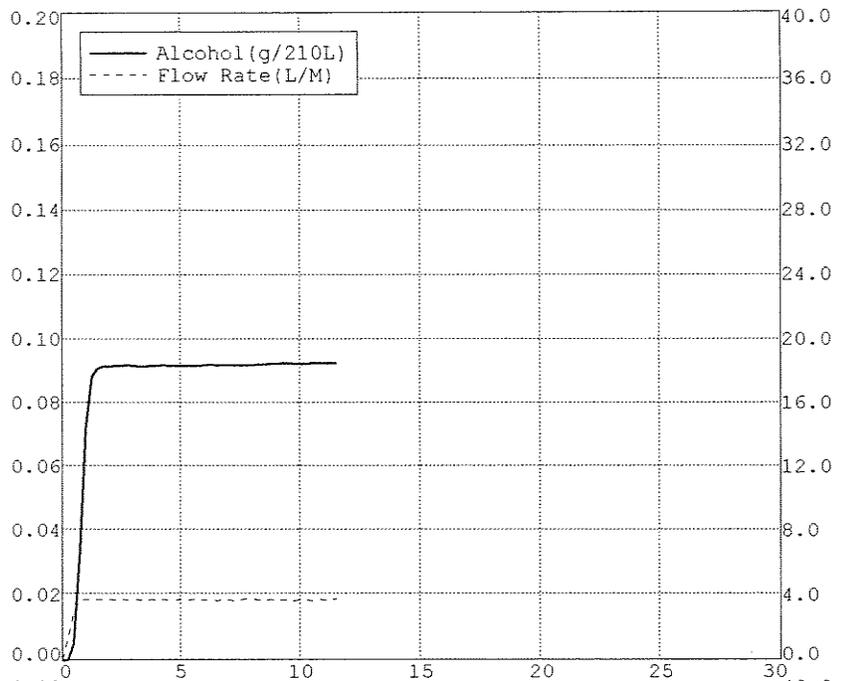

Charles B Geisler #296