

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 02/24/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:02
INTERNAL STANDARD	VERIFIED	00:02
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:02
BLANK TEST	0.00	00:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:03
BLANK TEST	0.00	00:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:05
BLANK TEST	0.00	00:05

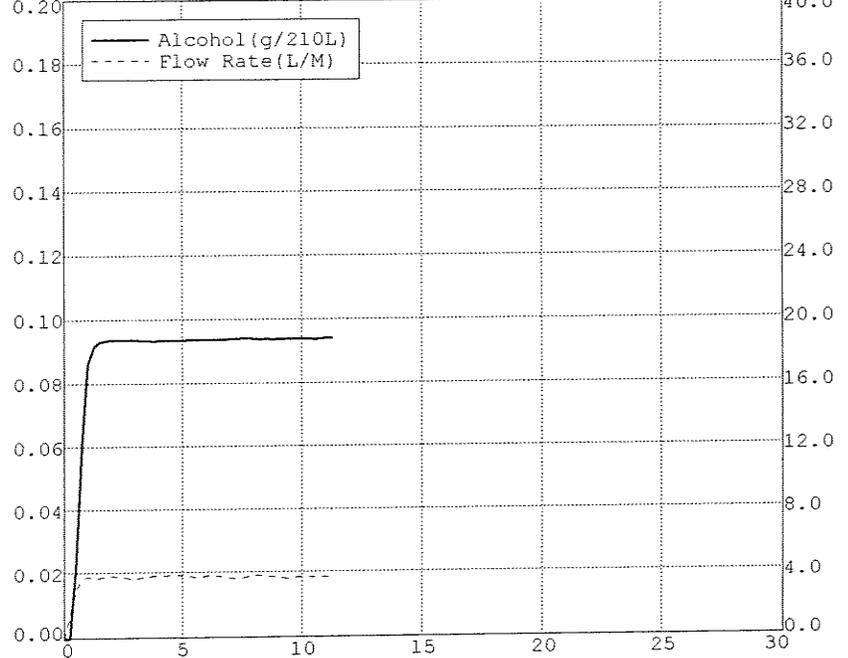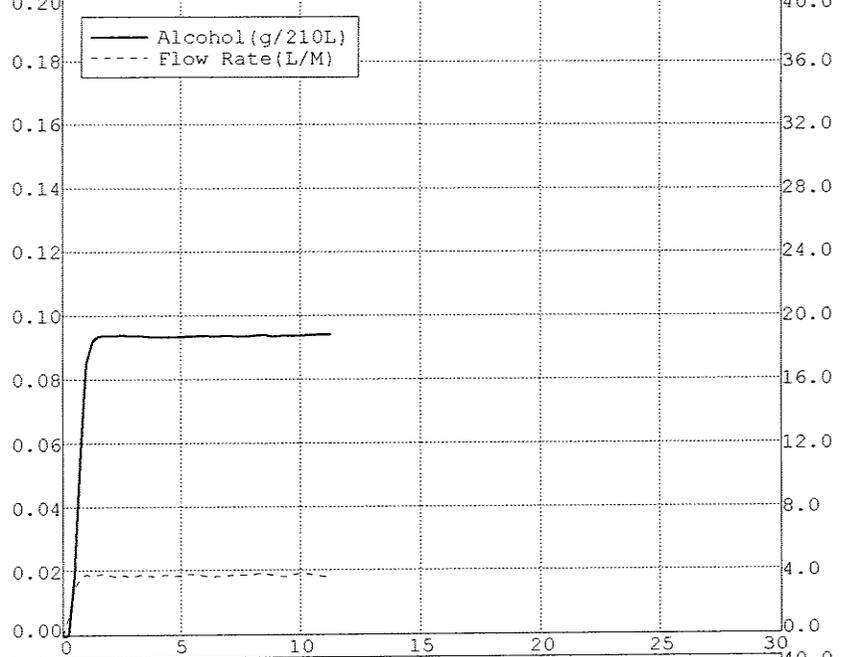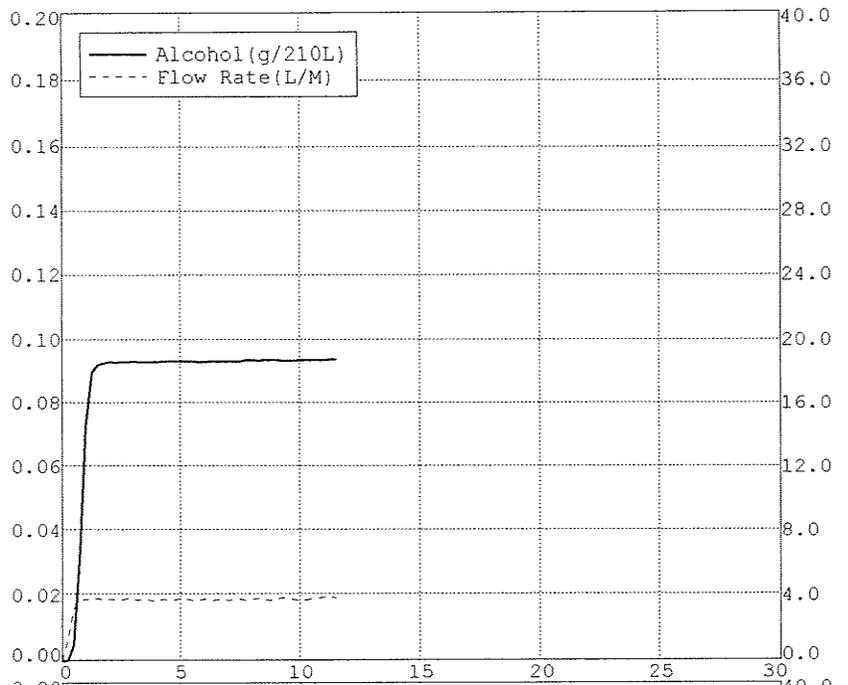

Charles B. Geisler #241