

SUPERVISOR TEST




WARREN COUNTY
SHERRIF'S OFFICE
DATAMASTER dmt: 144506

Date: 03/07/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:10
INTERNAL STANDARD	VERIFIED	03:11
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	03:11
BLANK TEST	0.00	03:12
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	03:12
BLANK TEST	0.00	03:13
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	03:13
BLANK TEST	0.00	03:14

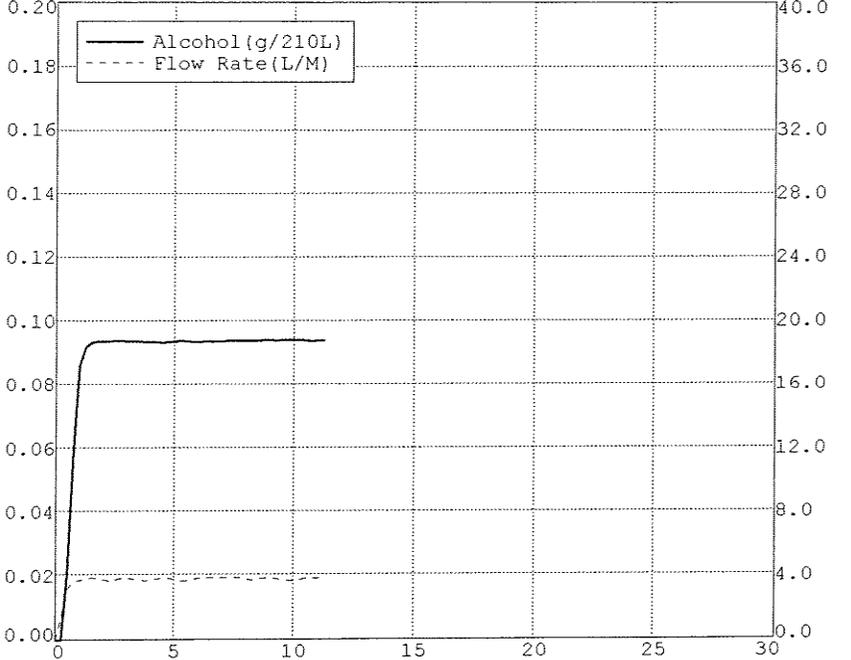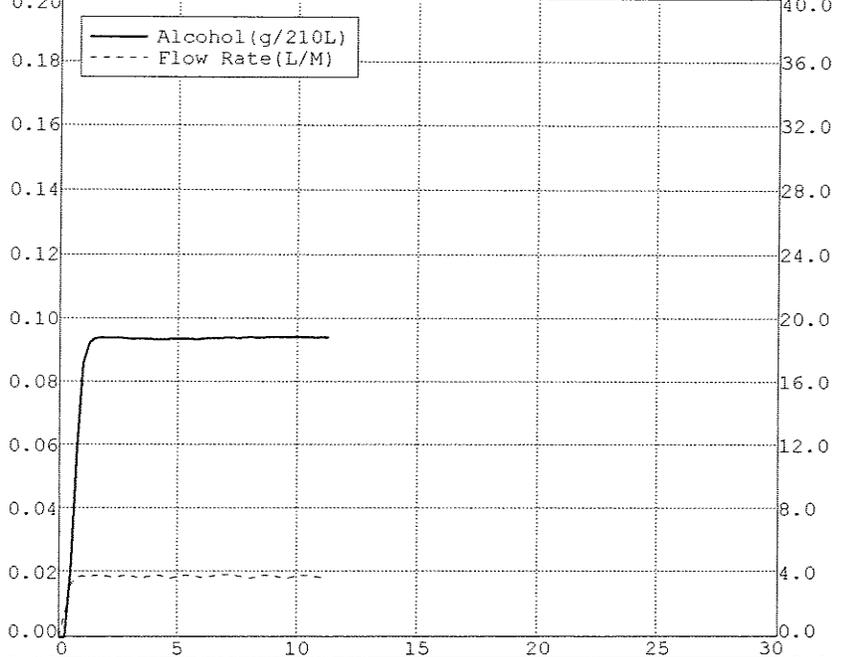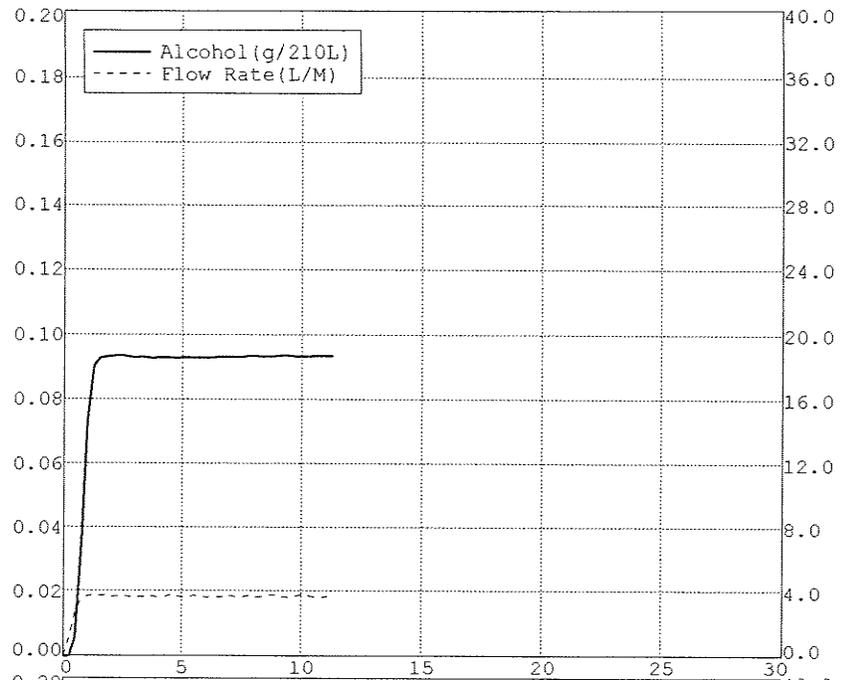

Charles B Geisler #441