

SUPERVISOR TEST




WARREN COUNTY  
 SHERRIF'S OFFICE  
 DATAMASTER dmt: 144506

Date: 03/15/2018

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:31
INTERNAL STANDARD	VERIFIED	02:31
REFERENCE STANDARD TEMP	34.04c	
REFERENCE STANDARD	0.09	02:32
BLANK TEST	0.00	02:32
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:33
BLANK TEST	0.00	02:34
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	02:34
BLANK TEST	0.00	02:35

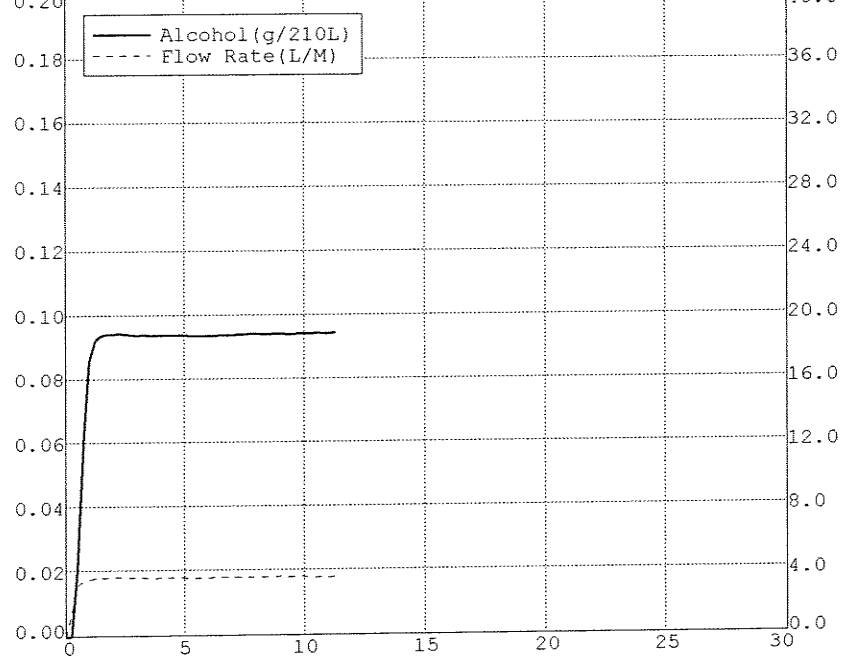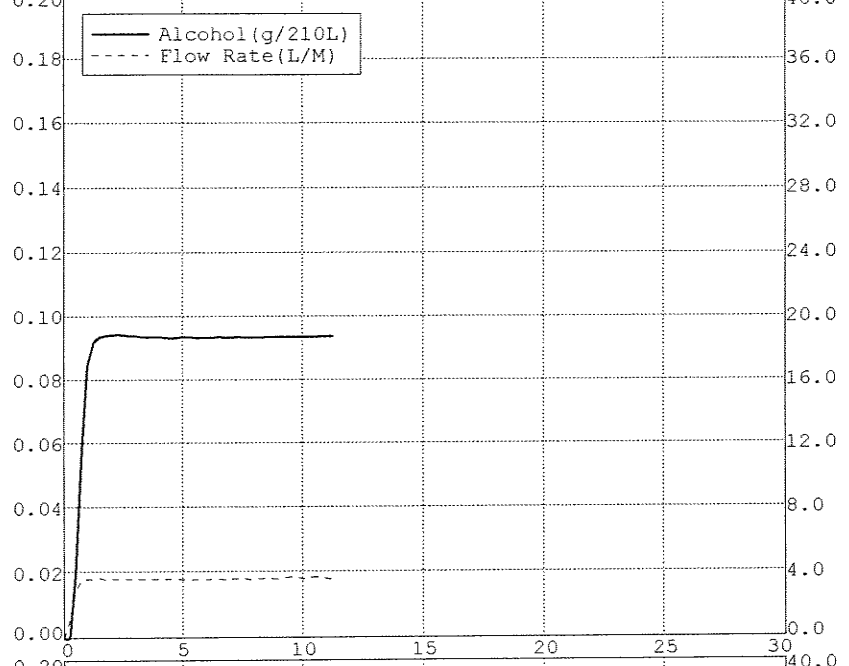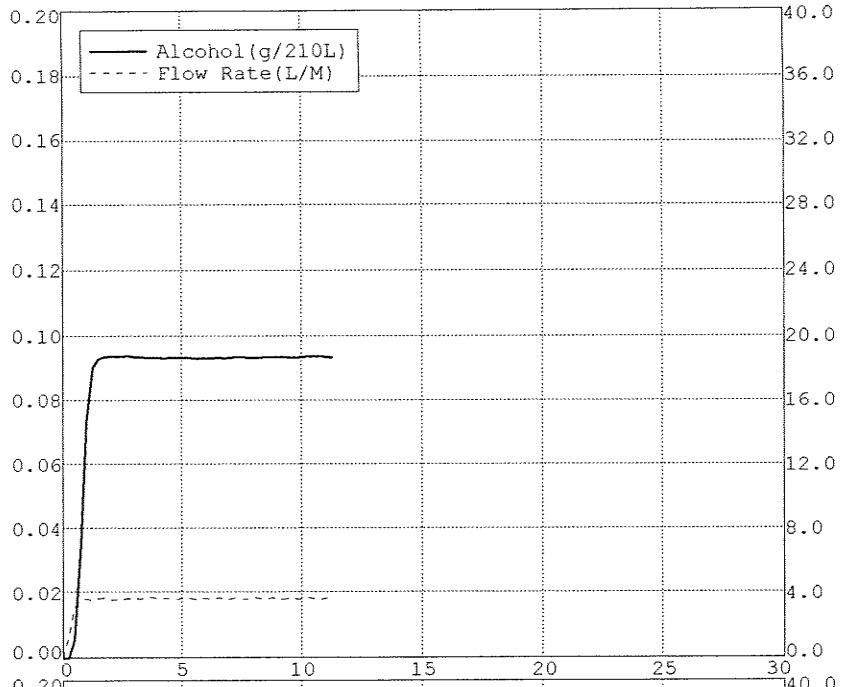

*Charles B. Geisler #215*