

SUPERVISOR TEST




WARREN COUNTY
SHERRIF'S OFFICE
DATAMASTER dmt: 144506

Date: 03/23/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:38
INTERNAL STANDARD	VERIFIED	23:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:38
BLANK TEST	0.00	23:39
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	23:39
BLANK TEST	0.00	23:40
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	23:40
BLANK TEST	0.00	23:41

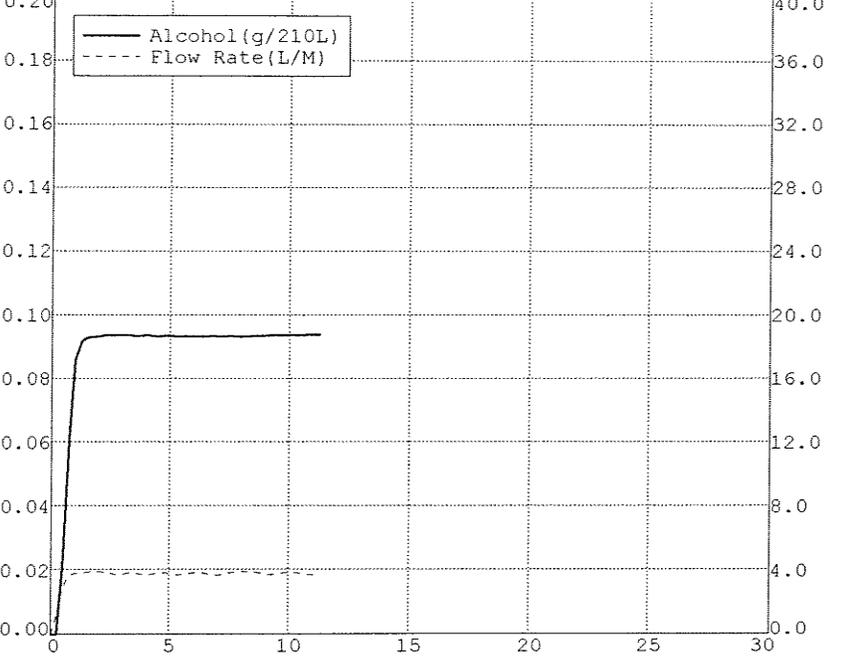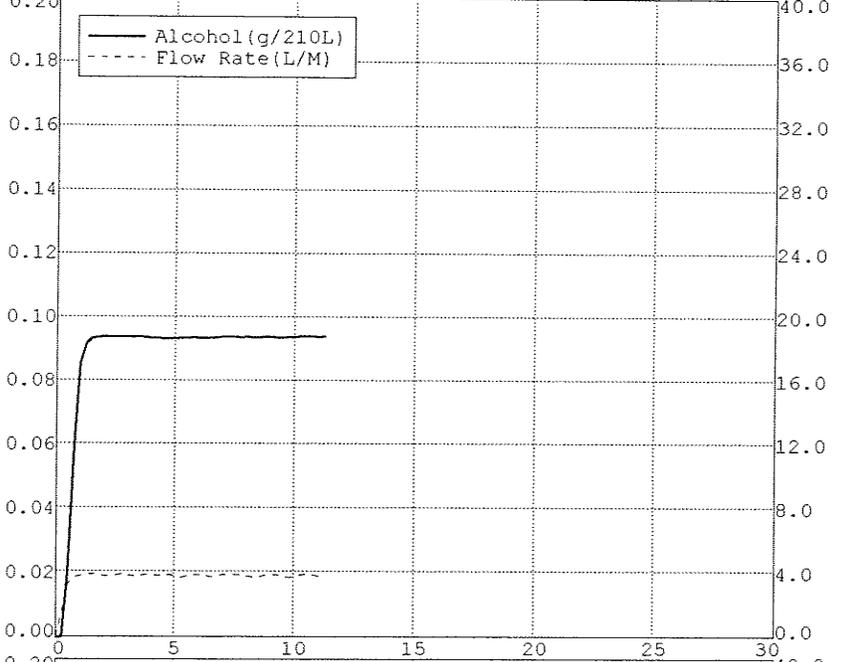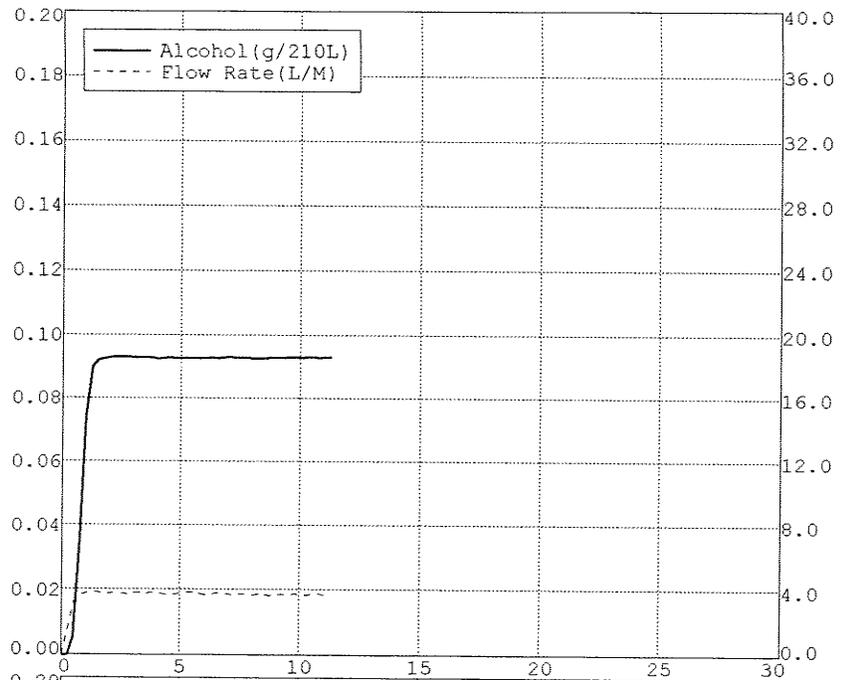

Charles B. Geisler