

SUPERVISOR TEST




WARREN COUNTY
SHERRIF'S OFFICE
DATAMASTER dmt: 144506

Date: 04/07/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:02
INTERNAL STANDARD	VERIFIED	01:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:03
BLANK TEST	0.00	01:03
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:04
BLANK TEST	0.00	01:05
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:05
BLANK TEST	0.00	01:06

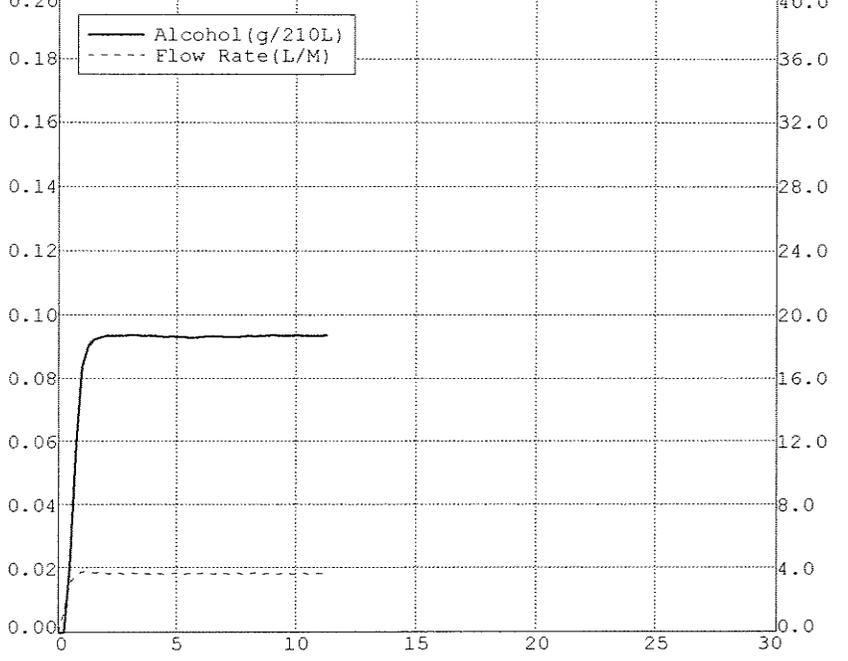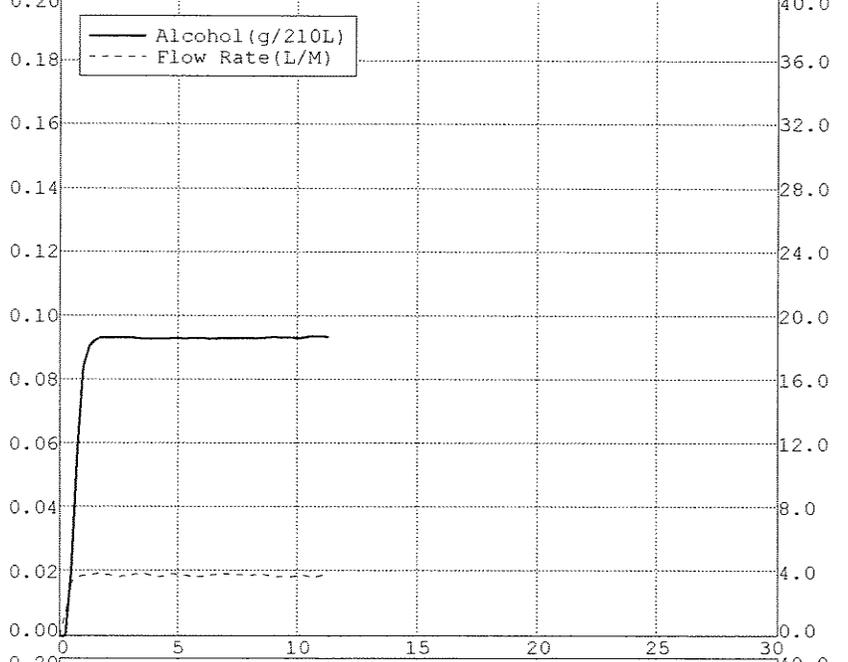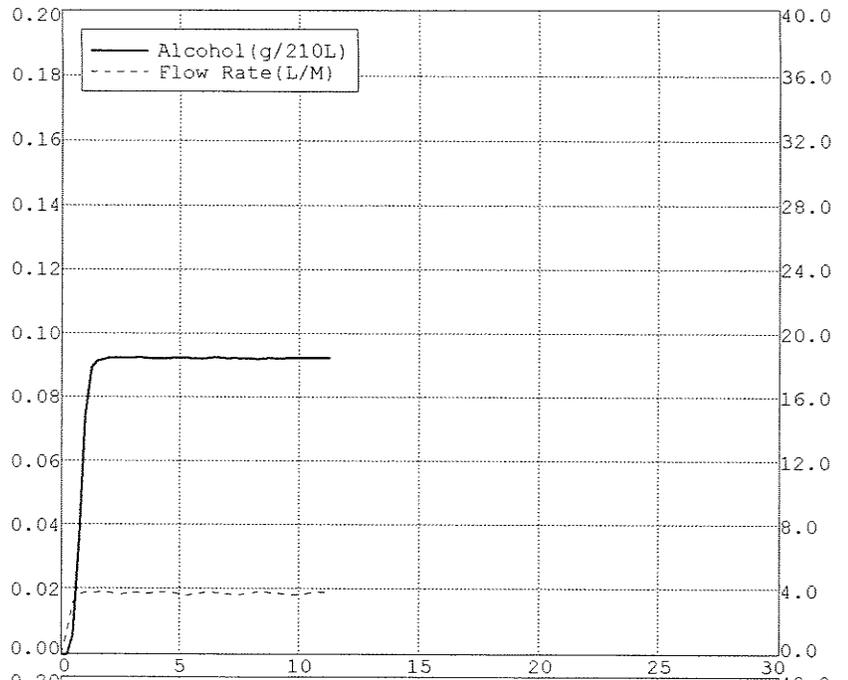

Charles B. Geisler #204