

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 04/13/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:04
INTERNAL STANDARD	VERIFIED	04:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	04:05
BLANK TEST	0.00	04:06
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	04:06
BLANK TEST	0.00	04:07
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	04:07
BLANK TEST	0.00	04:08

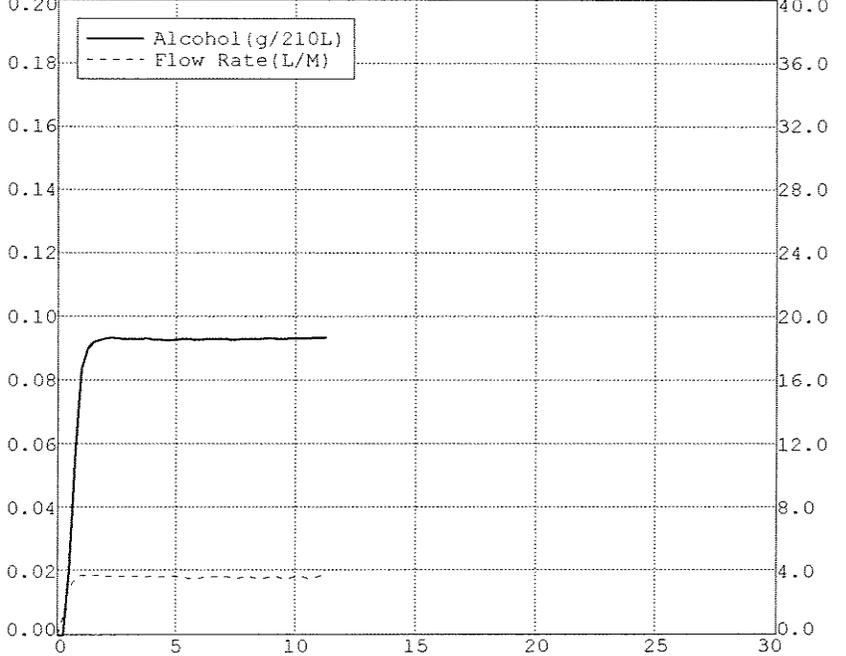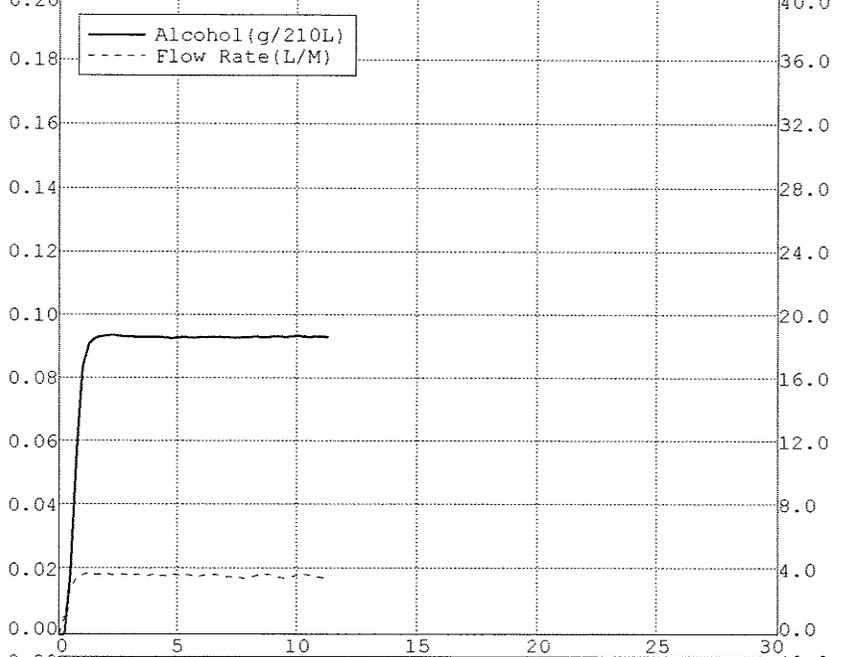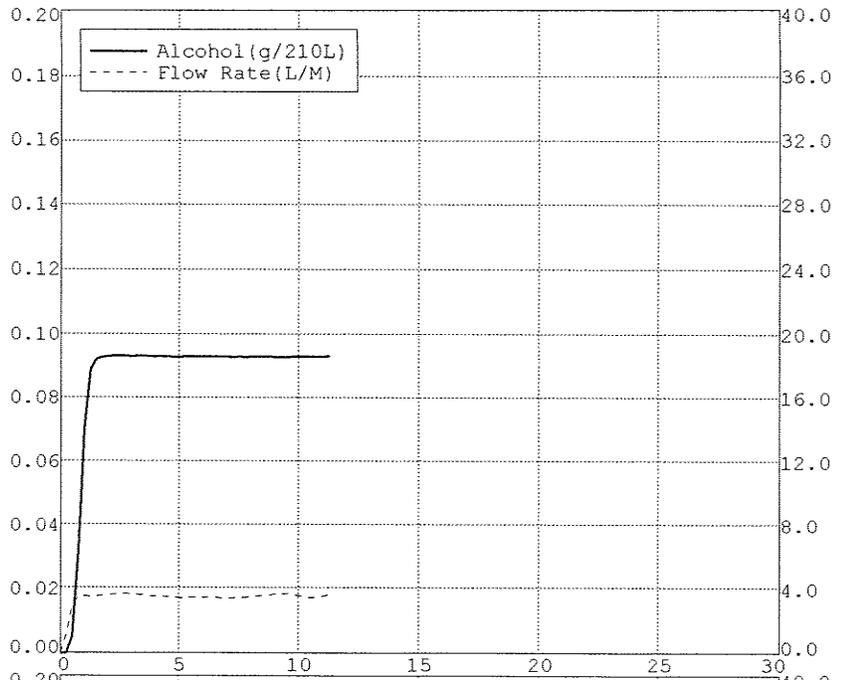

*Charles B. Geisler #291*