

SUPERVISOR TEST




WARREN COUNTY  
 SHERRIF'S OFFICE  
 DATAMASTER dmt: 144506

Date: 05/29/2018

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:03
INTERNAL STANDARD	VERIFIED	01:03
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:03
BLANK TEST	0.00	01:04
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	01:05
BLANK TEST	0.00	01:06
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:06
BLANK TEST	0.00	01:07

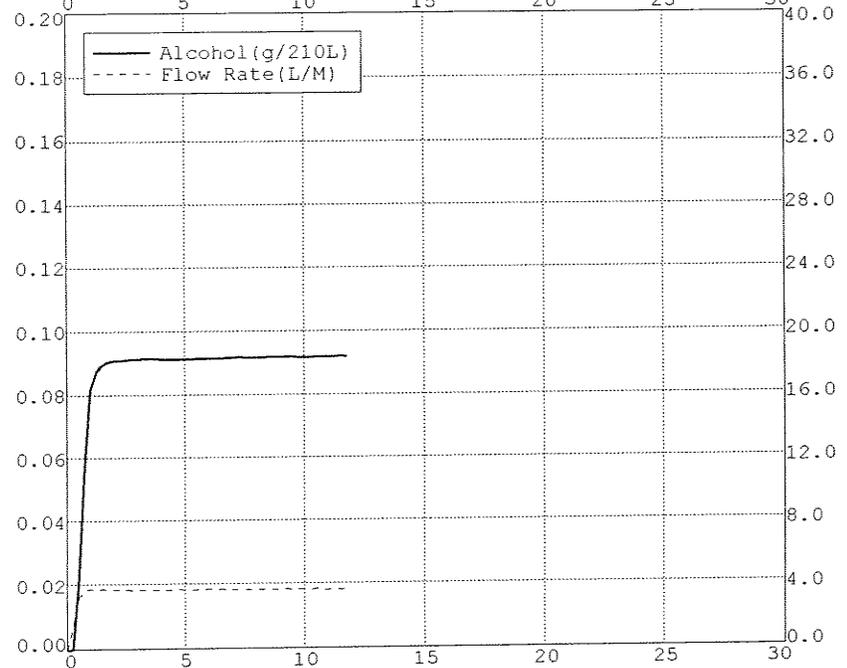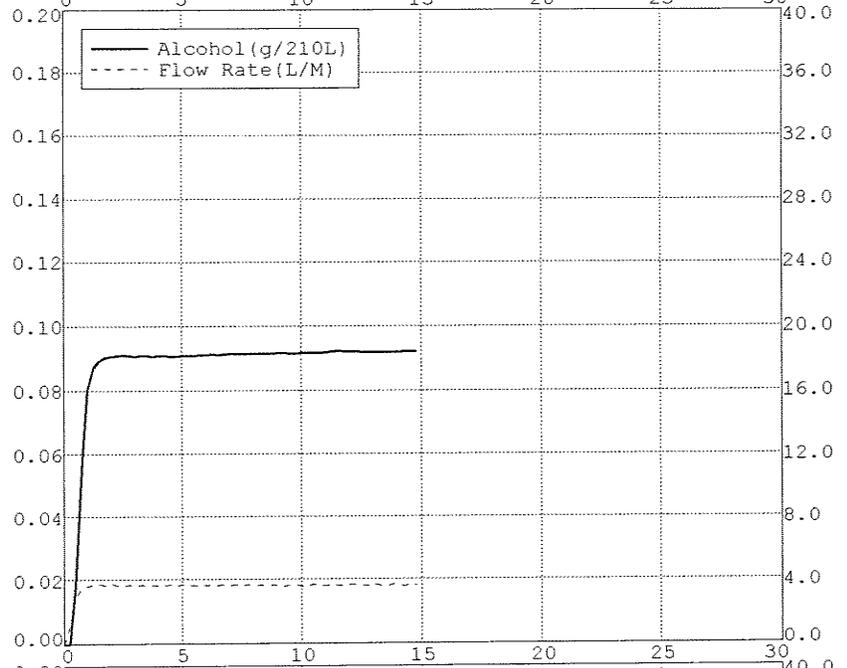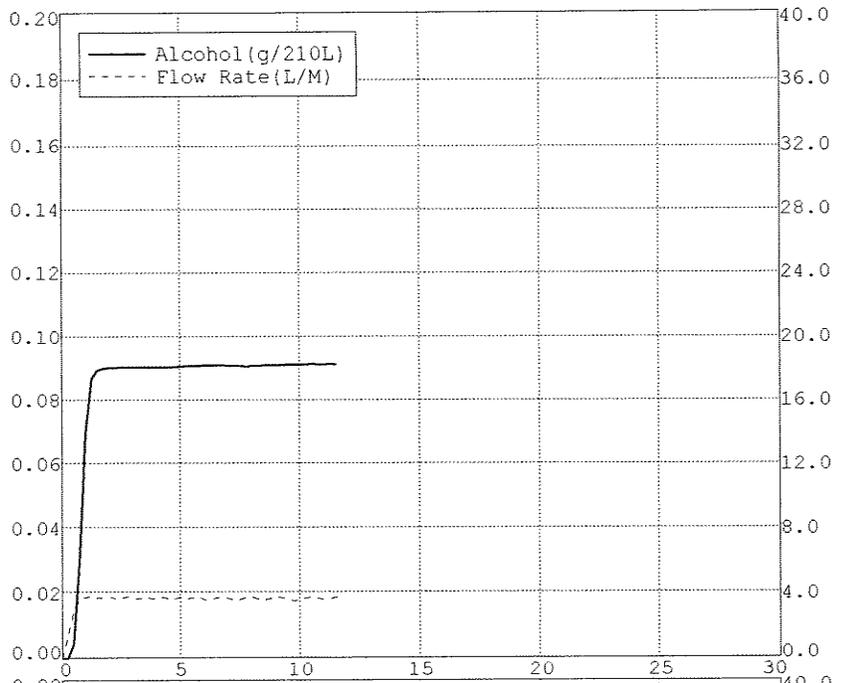

*Charles B. Geisler* #241