

SOLUTION CHANGE




WARREN COUNTY
 SHERRIF'S OFFICE
 DATAMASTER dmt: 144506

Date: 06/02/2018

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:04
INTERNAL STANDARD	VERIFIED	02:05
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:05
BLANK TEST	0.00	02:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:07
BLANK TEST	0.00	02:07
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	02:08
BLANK TEST	0.00	02:09

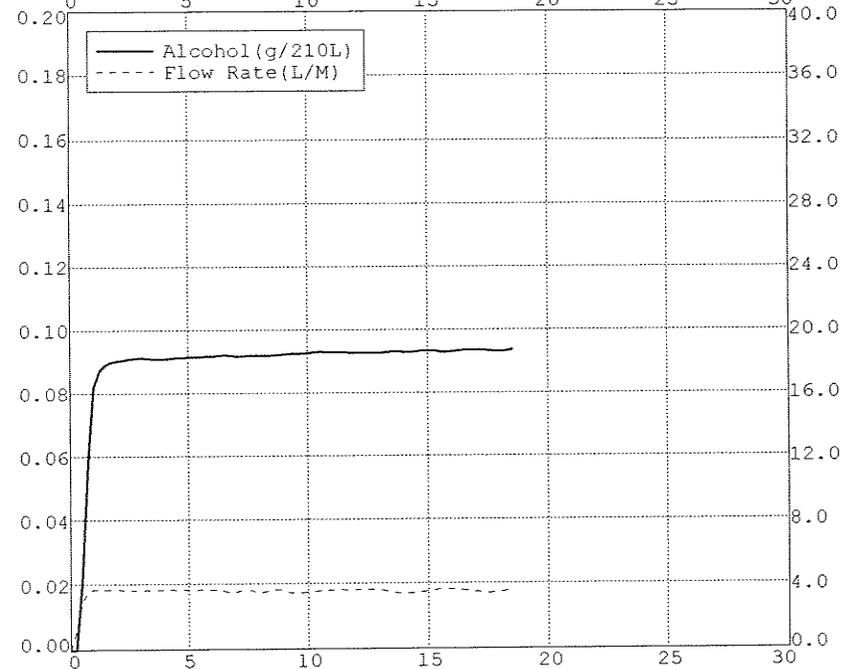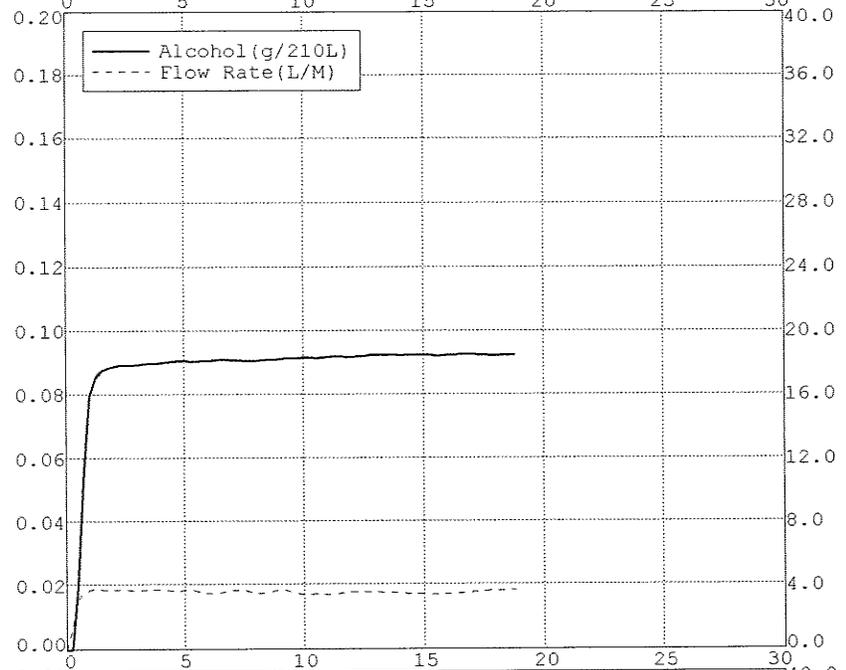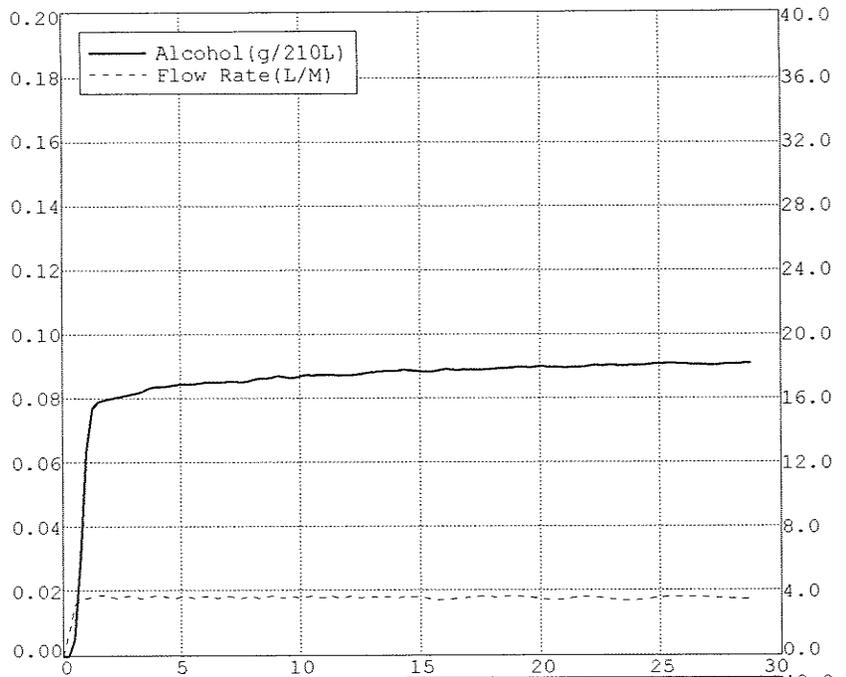

Charles B. Geisler