

SUPERVISOR TEST




WARREN COUNTY  
SHERRIF'S OFFICE  
DATAMASTER dmt: 144506

Date: 06/09/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:31
INTERNAL STANDARD	VERIFIED	21:31
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	21:32
BLANK TEST	0.00	21:33
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	21:33
BLANK TEST	0.00	21:34
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:34
BLANK TEST	0.00	21:35

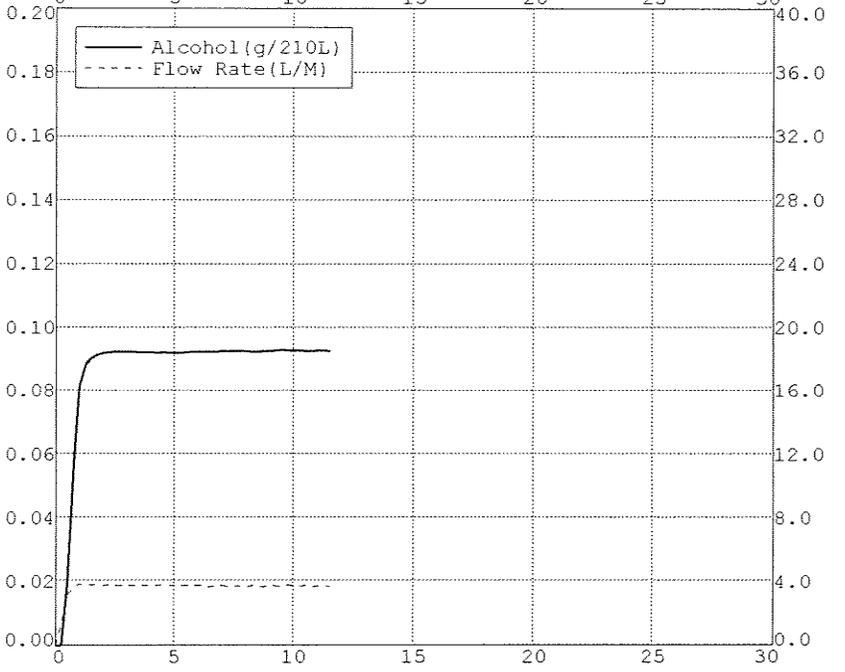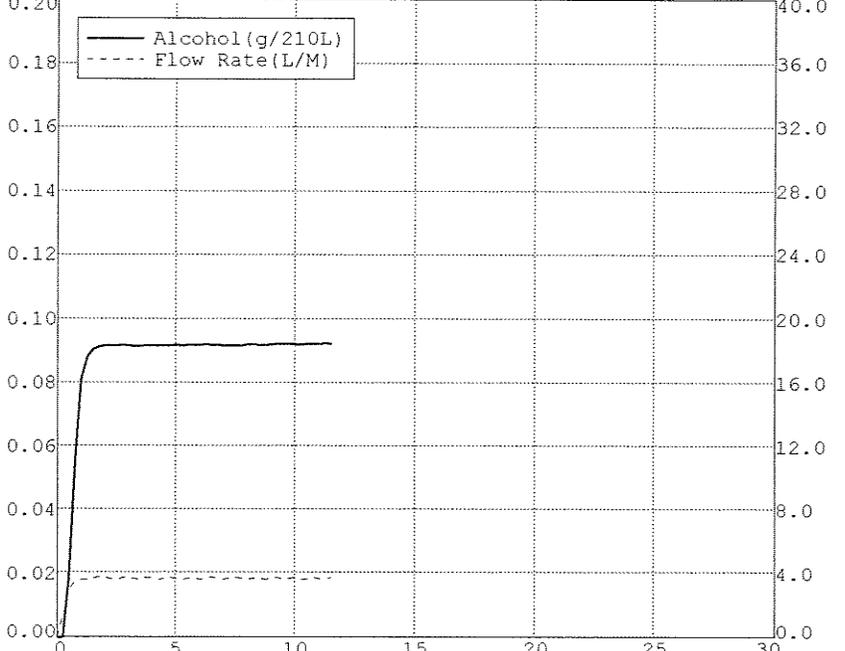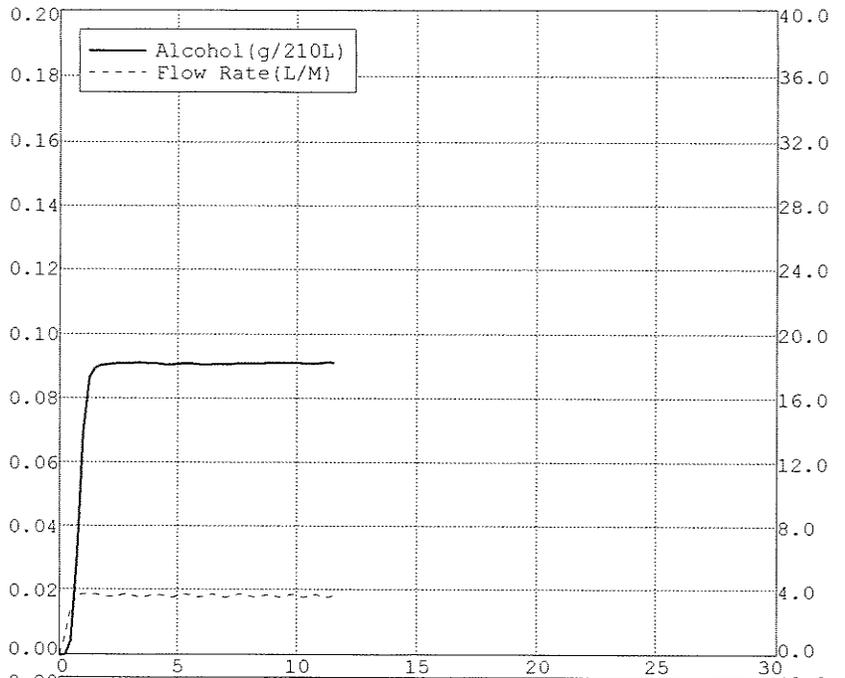

*Charles B Geisler* #20