

SUPERVISOR TEST




WARREN COUNTY  
SHERRIF'S OFFICE  
DATAMASTER dmt: 144506

Date: 06/16/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:33
INTERNAL STANDARD	VERIFIED	01:33
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:34
BLANK TEST	0.00	01:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:35
BLANK TEST	0.00	01:36
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:36
BLANK TEST	0.00	01:37

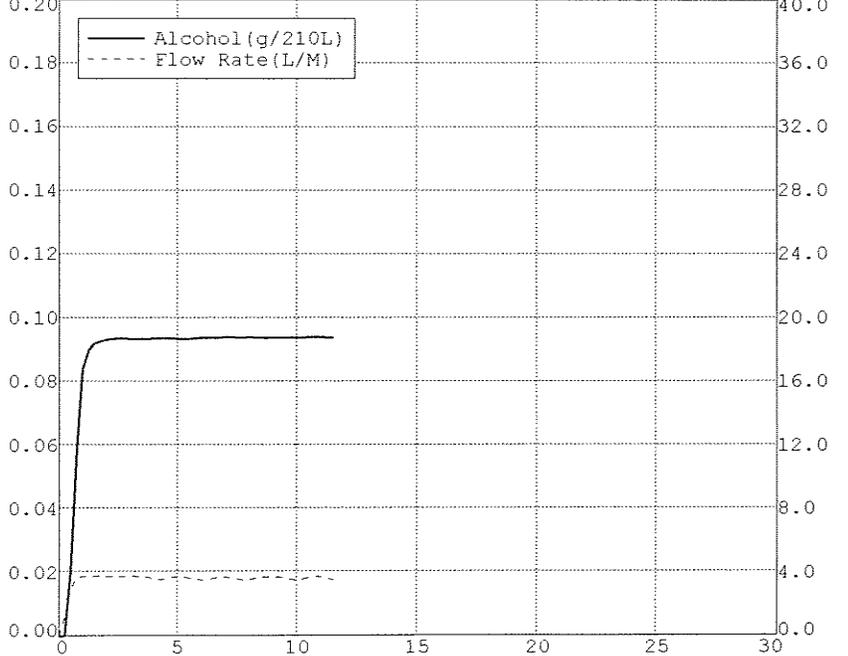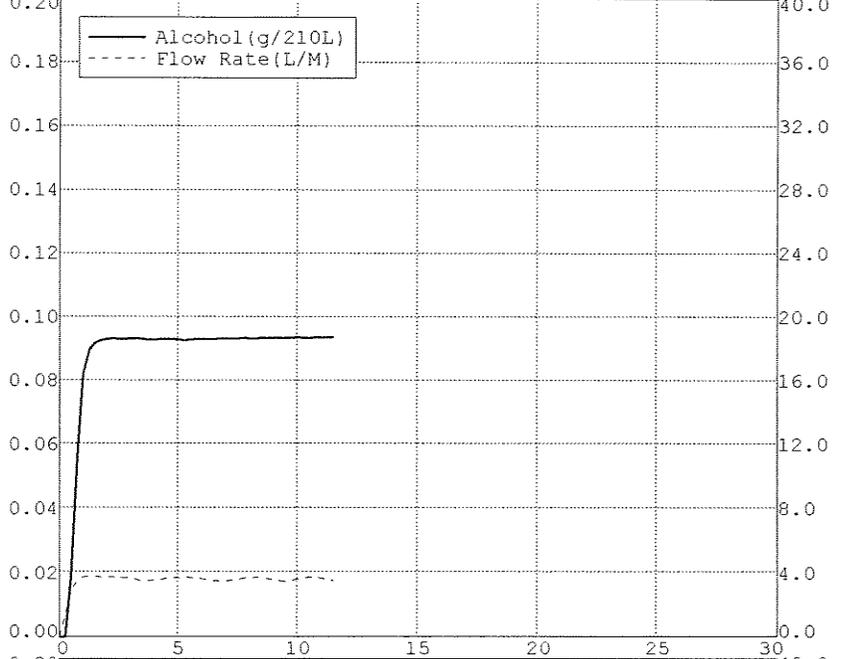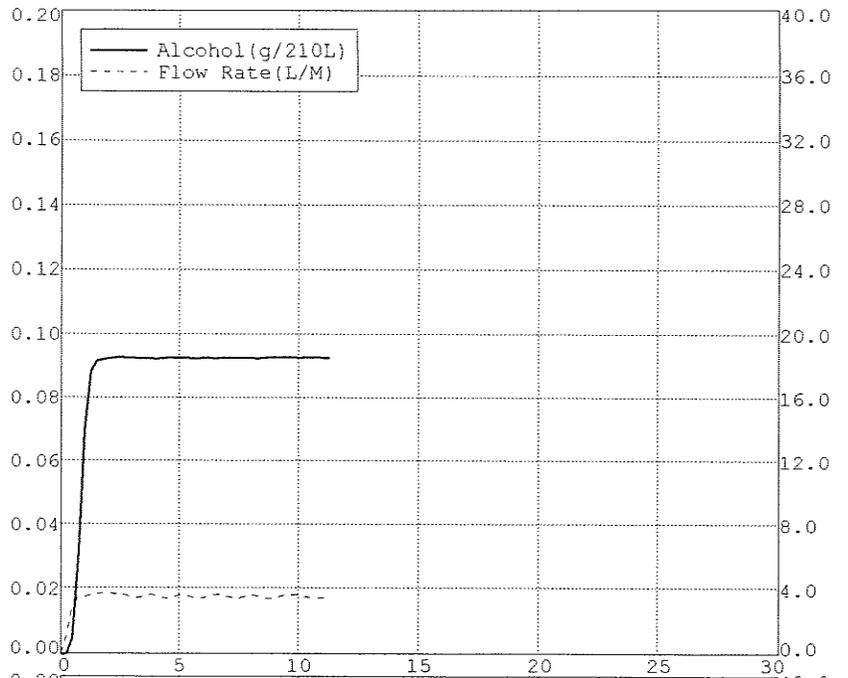

*Charles B. Geisler* #24