

SUPERVISOR TEST




WARREN COUNTY  
SHERRIF'S OFFICE  
DATAMASTER dmt: 144506

Date: 06/29/2018

OPERATOR NAME:  
RYAN C SCHROECK  
Permit #: 41316  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:17
INTERNAL STANDARD	VERIFIED	09:17
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:17
BLANK TEST	0.00	09:18
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	09:19
BLANK TEST	0.00	09:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:20
BLANK TEST	0.00	09:21

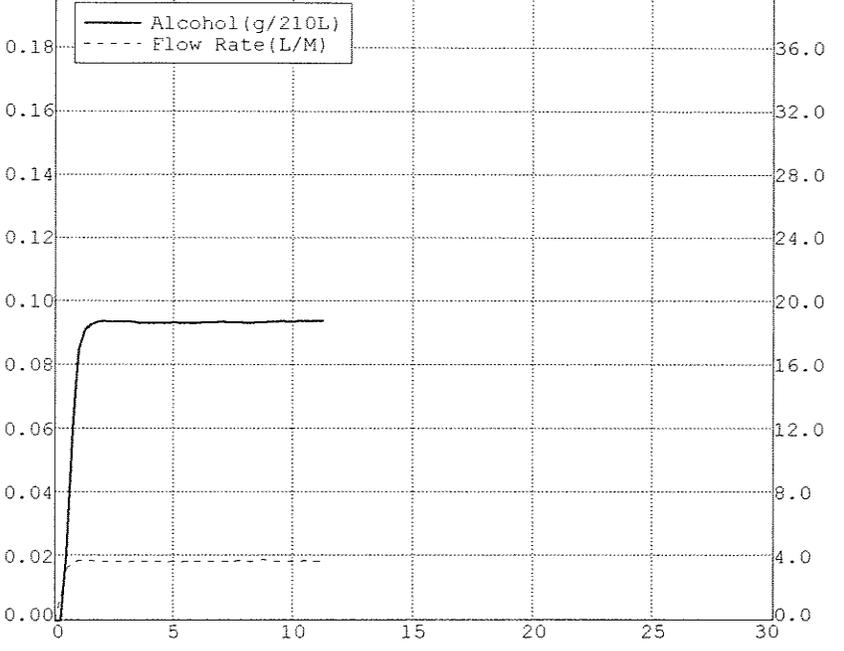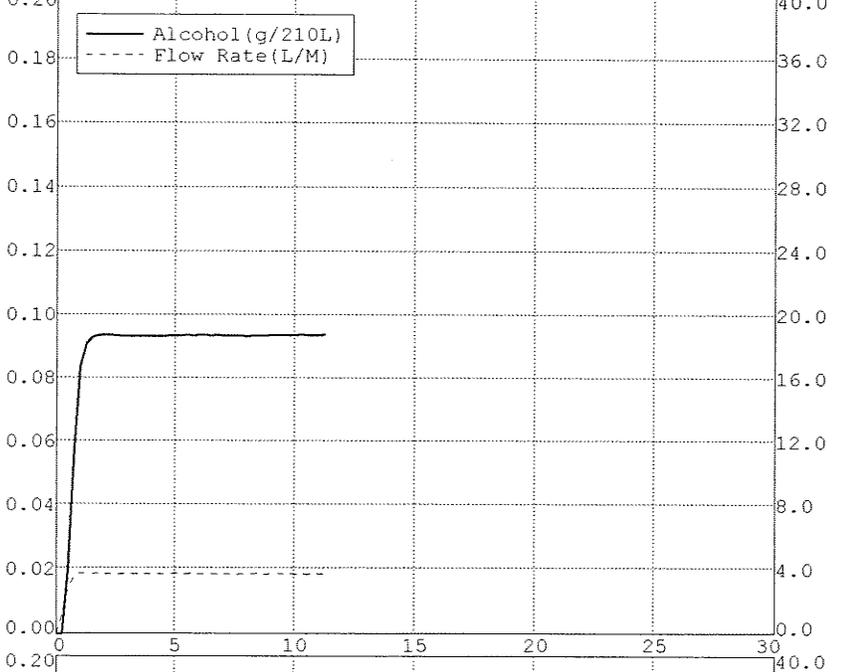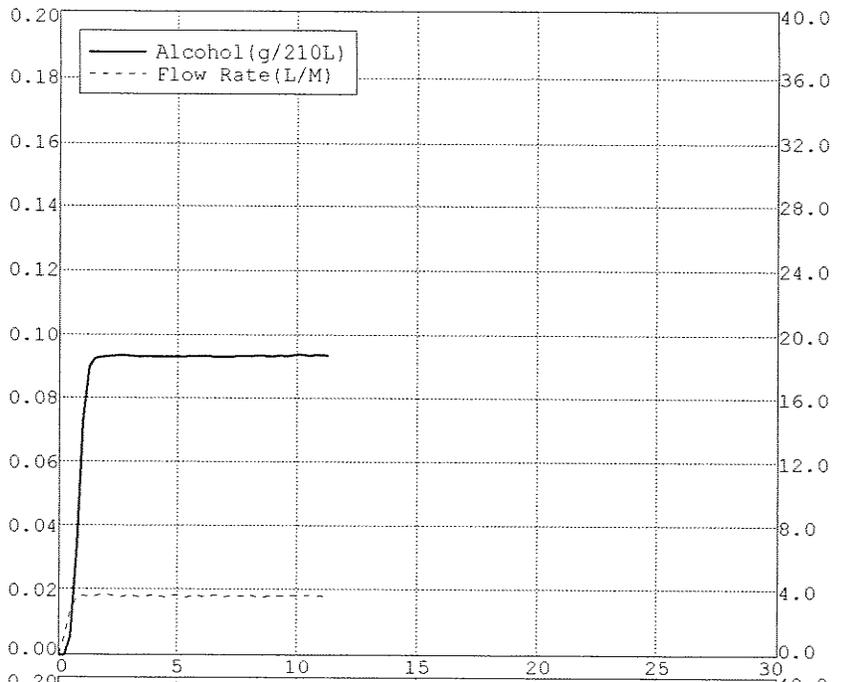

*Handwritten signature/initials*