

SUPERVISOR TEST




WARREN COUNTY  
SHERRIF'S OFFICE  
DATAMASTER dmt: 144506

Date: 07/29/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:52
INTERNAL STANDARD	VERIFIED	01:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:52
BLANK TEST	0.00	01:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:53
BLANK TEST	0.00	01:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:55
BLANK TEST	0.00	01:56

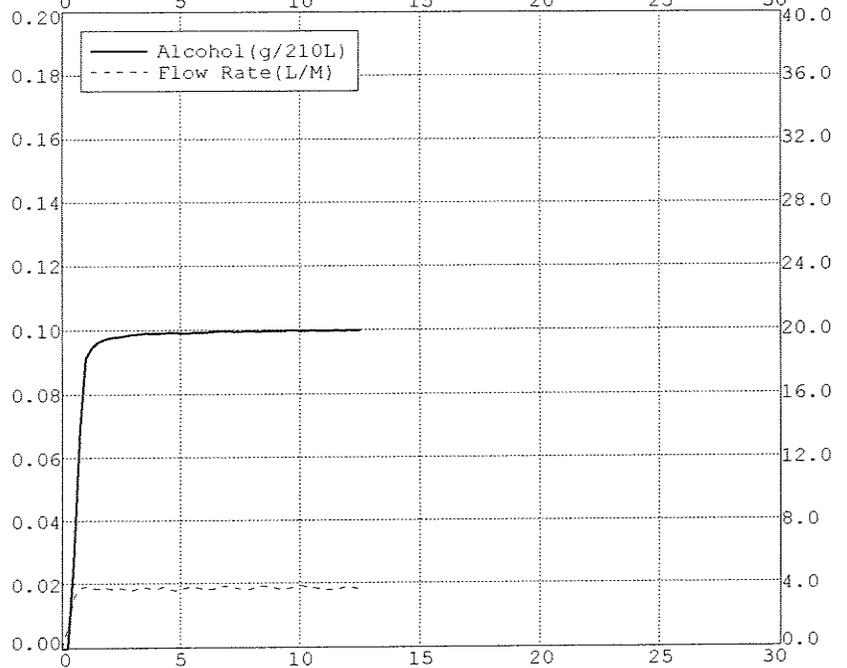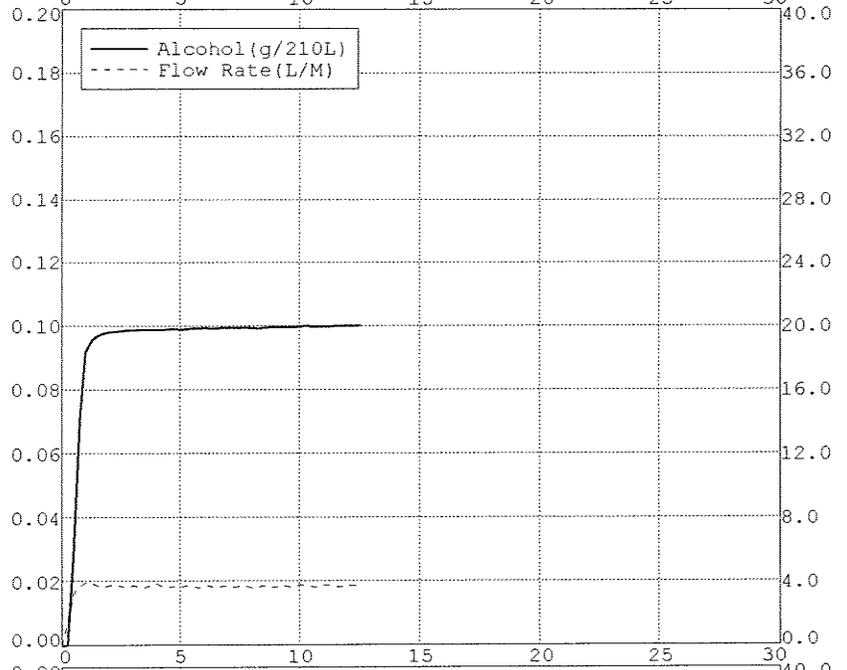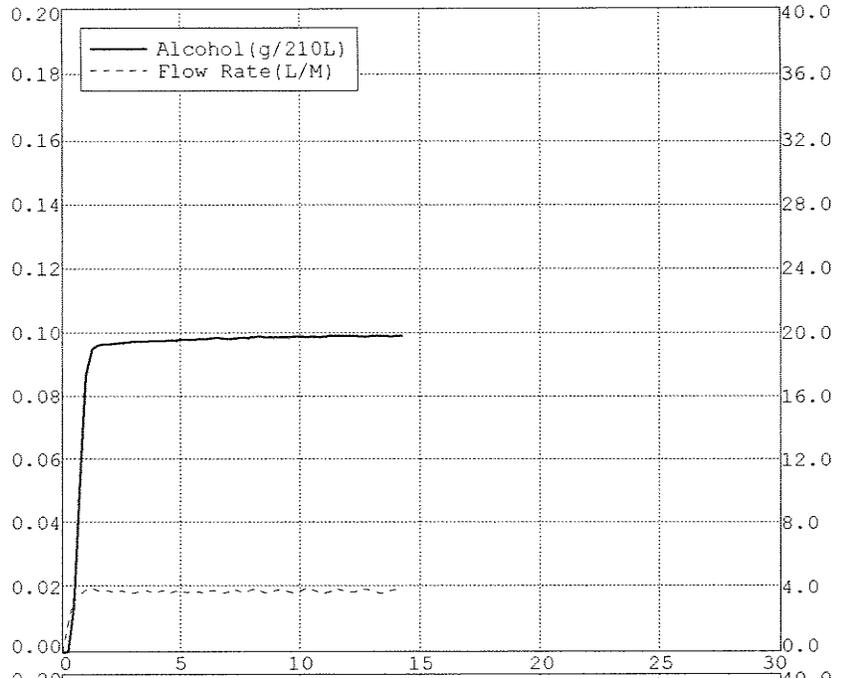

*Charles B. Geisler #201*