

SUPERVISOR TEST




WARREN COUNTY
SHERRIF'S OFFICE
DATAMASTER dmt: 144506

Date: 08/08/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18170

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:10
INTERNAL STANDARD	VERIFIED	00:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:10
BLANK TEST	0.00	00:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:12
BLANK TEST	0.00	00:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:13
BLANK TEST	0.00	00:14

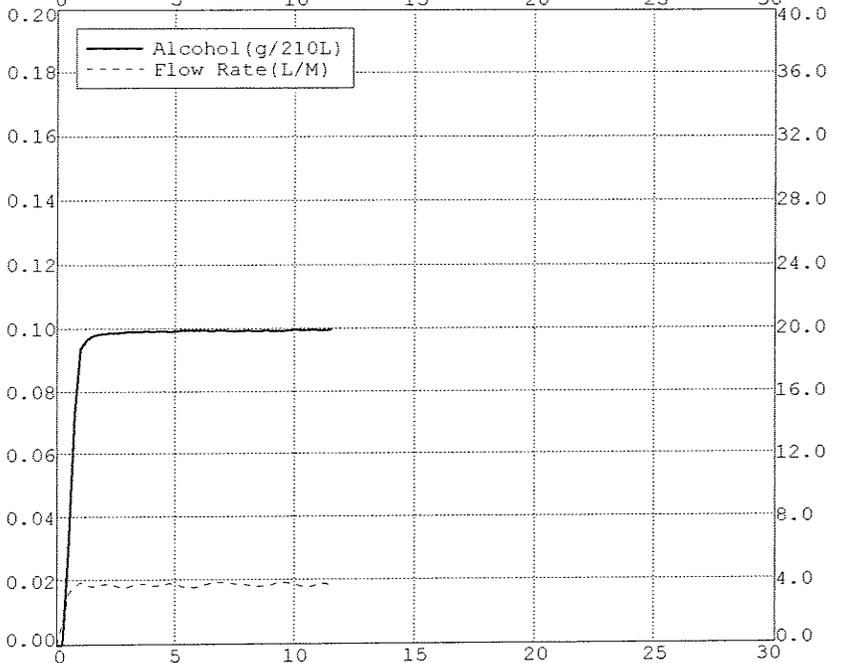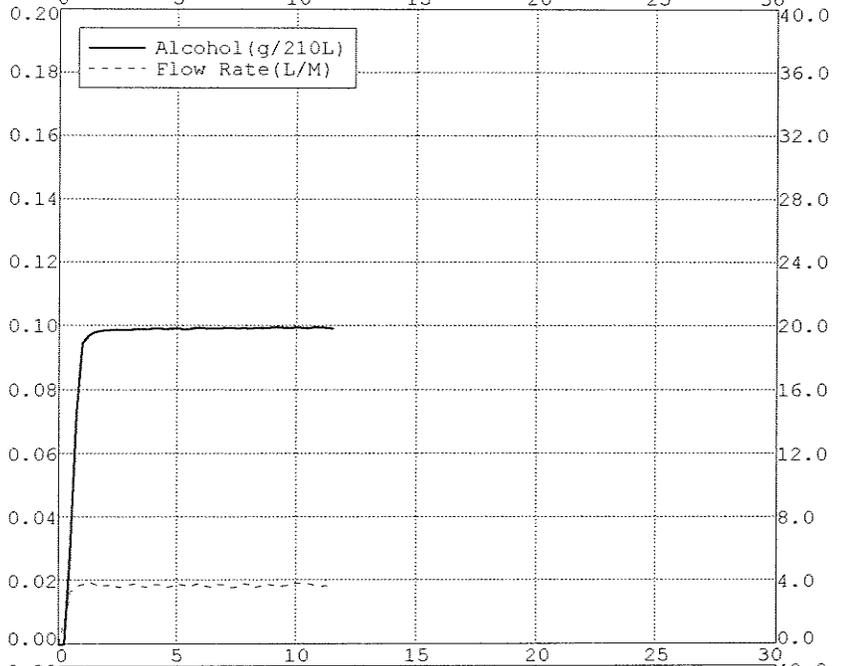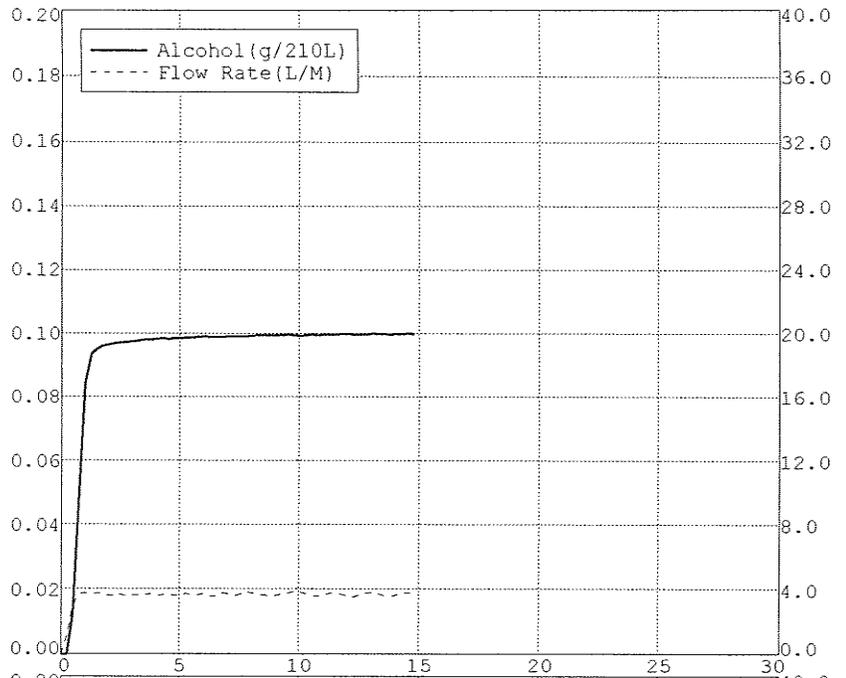

Charles B. Geisler #246